



# BEGO IMPLANT SYSTEMS

Product Catalogue

2021

Partners in Progress

 BEGO

**THERE FOR ME.  
BEGO IMPLANT SYSTEMS.**

---

Dear customers and partners

Teeth are essential for people's well-being – and replacing natural teeth is a major responsibility. Ensuring patients feel positive and safe with the assistance of our solutions for implant dentistry and bone regeneration has been motivating us for over 28 years.

**How we support you.**

As a family-run company, we put customer proximity and personal cooperation in first place.

Our comprehensive product range, the high safety level in production, manufacturing that is exclusively "made in Germany", and the high degree of reliability are good reasons to trust us and choose us as your partner.

You can rely on us – always.



## TABLE OF CONTENTS

---

<b>SERVICE</b>	<b>6</b>
BEGO – Solutions from a single source	6
SEMADOS CAMPUS	7
<b>REGENERATION · NATURESQUE</b>	<b>11</b>
naturesQue Regeneration Line	12
<b>SURGERY</b>	<b>15</b>
Descriptions and labels	16
Implant planning aids	19
BEGO Semados SC/SCX implants with Platform Switch design	21
BEGO Semados RS/RSX implants with Platform Switch design	25
BEGO Semados RI implants with Platform Switch design	29
Cover screws/healing abutments with Platform Switch design	31
<b>PROSTHETICS</b>	<b>65</b>
Instruments	66
<b>CAD/CAM Implant Prosthetics BEGO Medical</b>	<b>67</b>
• Interface overview	67
• Individual healing abutments	68
• Individual abutments	69
• Occlusally screw-retained bridge restorations	69
• Bar constructions	71
	72
<b>Prosthetics SC/SCX/RS/RSX/RI<sup>*1</sup> implants (PS<sup>*5</sup> design)</b>	<b>75</b>
• CAD/CAM restoration	75
• One Care Package restoration	76
• Impression taking and model fabrication	79
• Crown restoration Ø 3.0	80
• Crown and bridge restoration	81
• Multi <sup>Plus</sup> restoration	82
• Hybrid restoration	88
• Screws	92
	95
	95
<b>BEGO Implant Overview</b>	<b>8</b>
	7
<b>BEGO Semados S implants with Platform Match design</b>	<b>35</b>
Cover screws/healing abutments with Platform Match design	37
BEGO Semados Mini implants/healing abutments	39
BEGO Semados Provisional Implant System	41
BEGO Guide guided surgery	45
Preparation instruments	53
<b>Prosthetics S implants (PM<sup>*7</sup> design)</b>	<b>97</b>
• CAD/CAM restoration	98
• Impression taking and model fabrication	100
• Crown and bridge restoration	101
• Multi <sup>Plus</sup> restoration	106
• Hybrid restoration	110
• Screws	103
<b>Prosthetics Mini implants</b>	<b>115</b>
• CAD/CAM restoration	116
• Impression taking and model fabrication	116
• Crown restoration	117
• Hybrid restoration	118
• Screws	121

## TABLE OF CONTENTS

---

<b>DEMO MODELS/MATERIAL</b>	<b>123</b>		
Large-scale models	<b>124</b>	Demonstration material	<b>125</b>
<b>USEFUL INFORMATION</b>	<b>129</b>		
Torque specifications	<b>128</b>	Index by article numbers	<b>138</b>
Material specifications	<b>130</b>	Alphabetical index	<b>152</b>

**Note:** Depending on regulatory approvals, under some circumstances not all offered products or services are available in all countries.  
Please contact your local BEGO Implant Systems sales partner.

Images and illustrations are examples only and the colors, symbols, design and specifications on the labels and/or packages shown may deviate from real products.

Specifications for lengths and diameters may be rounded up or down for simplification.

Our products are constantly being refined. We therefore reserve the right to make changes.

© 2020 by BEGO Implant Systems GmbH & Co. KG, Bremen. We reserve all rights to reprints of extracts, photomechanical reproduction and particularly translations.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> Platform Switch design

\*<sup>7</sup> Platform Match design


## Solutions from a single source



### Conventional solutions

BEGO Bremer Goldschägerei GmbH & Co. KG develops and sells precious metal and non-precious metal dental alloys and provides equipment, materials and services for fabricating premium dental restorations. The company also offers ceramics for further processing in the dental laboratory.

Since its founding, and now moving into its fifth generation, BEGO has realized its aim of providing dental laboratories with innovative and cost-effect products and services for optimal treatment of their patients, all from a single source.

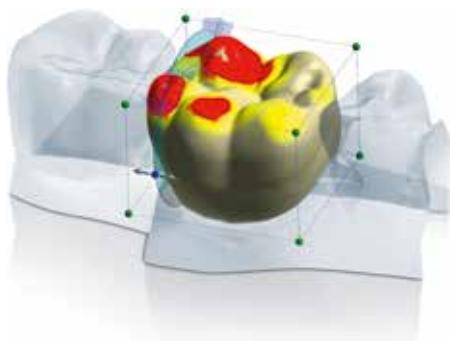

### CAD/CAM solutions

BEGO Medical GmbH specializes in digital processes and is a pioneer in CAD/CAM technology in the dental sector. The company is the inventor and holder of the patent for the Selective Laser Melting (SLM) procedure in the dental sector. All-round procedural expertise and the widest choice of materials ensure premium quality across many indications.

In its high-tech production centre located in Bremen, BEGO fabricates frameworks, abutments, crowns and bridges based on virtual models using the latest laser and milling techniques in four different procedures: SLM, High Speed Cutting (HSC), CAD/Cast® and Rapid Prototyping.



### Implant dentistry solutions

Since 1990 BEGO Implant Systems GmbH & Co. KG has been developing and fabricating dental implants and supplementary products to treat patients with implants around the world. An innovative 3D implant design, system abutments for modern implant dentistry, a safe biomaterials system, and functionally optimized guided surgery all mean that dental implants "Made by BEGO" lead to planned and reproducible results. These are premium German products that incorporate technological progress with fair prices, combining safety, durability, aesthetics and reliability.



### BEGO TRAINING CENTER

Practical knowledge of subjects such as CAD/CAM or traditional dental technology are taught by an internationally experienced team of trainers in courses – both for beginners and advanced users – that are specifically tailored to meet the most diverse requirements.

Our in-house course concepts form the basis of a challenging program for seminars and practical courses that help motivated dental technicians become even more successful.

## Professional development: A focus of BEGO Implant Systems SEMA DOS CAMPUS

Supporting postgraduate dental training and qualification of dental technicians in the area of modern, implant-retained prosthetics is the focus of BEGO Implant Systems – and has been right from the start.

So that we can continuously optimize our training programs, we have formed a number of framework agreements with various national and international professional development training centres under the umbrella brand SEMADOS CAMPUS. You can read about our international training programs in our course brochure. Our website also has more information about the latest courses on offer.

For international training programs, please contact our worldwide sales partners or contact BEGO Implant Systems in Bremen directly.

For professional development courses for dental technicians, academia dental® (<http://www.academia-dental.de>) and the BEGO TRAINING CENTER (<http://www.bego.com/de/fortbildung/bego-training-center/>) in Bremen are available.

Is there a course or training program you'd like to see offered? We happily accept any suggestions you may have.

# SEMA DOS Campus

## MANY PATIENTS, MANY SOLUTIONS

### Parallel implant shape

Those who want to treat their patients based on needs require comprehensive treatment solutions. Our implant systems are highly suited for many areas of application.

Self-tapping

SC/SCX implants  
page 21  
S implants  
page 36



### Conical implant shape

The implants have a conical inner connection with a mean conical angle of 45° as well as an internal hex that acts as an anti-rotation mechanism (does not apply for Mini and PI).

Self-tapping

Condensing

RI implants  
page 30



### Provisional implants

Provisional implants  
page 42



### You have the choice

Individual for each patient down to the last detail – BEGO Semados® S/SC/SCX

#### S Implant

- Machined implant shoulder
- Platform Match design
- Fully guided surgery is an option

#### SC Implant

- Machined implant shoulder
- Platform Switch design
- Fully guided surgery is an option

#### SCX Implant

- Micro-structured implant shoulder
- Platform Switch design
- Fully guided surgery is an option

### Fits just about every time

Depending on preference – BEGO Semados® RS/RSX

#### RS Implant

- Machined implant shoulder
- Platform Switch design
- Fully guided surgery is an option

#### RSX Implant

- Micro-structured implant shoulder
- Platform Switch design
- Fully guided surgery is an option

### Cuts a fine figure

For primary and long-term stability – BEGO Semados® RI

#### RI Implant

- Machined implant shoulder
- Platform Switch design
- Guided surgery is an option

### Mini done differently

For narrow jaws and small spaces – BEGO Semados® Mini

#### Mini Implant

- Machined implant shoulder
- Large selection of prosthetic solutions available, including tension-free CAD/CAM-fabricated bar constructions

### Firm fit for in-between

Stabilization during the healing phase – BEGO Semados® PI

#### PI Implant

- Relieves loads on augmented areas and the soft tissue
- Untreated machined surface
- Best possible alignment thanks to the malleable implant neck





## OVERVIEW

naturesQue Regeneration Line

12

## REGENERATION · NATURESQUE

naturesQue Regeneration Line				
Description	REF	Specification	Container	Contents
<b>naturesQue MaxOss P</b> porcine bone substitute material	58488	0.25–1.0mm	Jar	0.5ml
	58489	0.25–1.0mm	Jar	1.0ml
	58490	0.25–1.0mm	Jar	2.0ml
	58491	0.25–1.0mm	Jar	4.0ml
	58492	1.0–2.0mm	Jar	1.0ml
	58493	1.0–2.0mm	Jar	2.0ml
	58494	0.25–1.0mm	Syringe	0.25ml
	58495	0.25–1.0mm	Syringe	0.5ml
<b>naturesQue SemOss B</b> Xenohybrid bovine bone substitute material	58500	0.25–1.0mm	Vial	0.25g; 0.5ml
	58501	0.25–1.0mm	Vial	0.5g; 1.0ml
	58502	0.25–1.0mm	Vial	1.0g; 2.0ml
	58503	0.25–1.0mm	Vial	2.0g; 4.0ml
	58504	1.0–2.0mm	Vial	0.5g; 1.0ml
	58505	1.0–2.0mm	Vial	1.0g; 2.0ml
	58506	1.0–2.0mm	Vial	2.0g; 4.0ml
<b>naturesQue ColTect P</b> porcine barrier membrane	58496	15 × 20mm	Piece	1
	58497	20 × 30mm	Piece	1
	58498	30 × 40mm	Piece	1
<b>naturesQue ColAid B</b> bovine collagen microfibrils	58499	0.1g	Vial	15
<b>naturesQue ColAid P</b> porcine collagen fleece	58507	20 × 20mm	Piece	10

BEGO Biomaterials* <sup>1</sup>				
Description	REF	Specification	Container	Contents
<b>BEGO Collagen Membrane</b> porcine barrier membrane	57221	15 × 20mm	Piece	1
	57222	20 × 30mm	Piece	1
	57223	30 × 40mm	Piece	1

**Note:** Depending on regulatory approvals, not all naturesQue products are available in all countries.  
Please contact your local BEGO Implant Systems sales partner.  
Returns and exchanges are not possible because of the temperature sensitivity of these products.

\*<sup>1</sup> as long as stocks last

[Duck]  
synonymous with empathy,  
trust, and respect

# naturesQue

»  
**REGENERATION  
MATERIALS**



naturesQue Regeneration Materials  
combines the strengths of the  
products' natural origins with  
scientific and clinical expertise for  
tissue regeneration.

## The essence of nature in expert hands.

**BEGO IMPLANT SYSTEMS**

Partners in Progress

[www.bego.com](http://www.bego.com)

 **BEGO**





## OVERVIEW

Descriptions and labels	16
Implant planning aids	19
BEGO Semados® SC/SCX implants with Platform Switch design	21
BEGO Semados® RS/RSX implants with Platform Switch design	25
BEGO Semados® RI implants with Platform Switch design	29
Cover screws/healing abutments with Platform Switch design	31
BEGO Semados® S implants with Platform Match design	35
Cover screws/healing abutments with Platform Match design	37
BEGO Semados® Mini implants/healing abutments	39
BEGO Semados® Provisional Implant System	41
BEGO Guide guided surgery	45
Preparation instruments	53

## Platform Switch



## Platform Match and external hex



## The BEGO Semados® implant family

### Platform Switch implants

#### SC implant

self-tapping, cylindrical implant  
with 0.5mm machined implant shoulder

#### SCX implant

self-tapping, cylindrical implant  
with 0.1mm machined implant shoulder

#### RS implant

self-tapping, conical implant  
with 0.5mm machined implant shoulder

#### RSX implant

self-tapping, conical implant  
with 0.1mm machined implant shoulder

#### RI implant

self-condensing, conical implant  
with 0.5mm machined implant shoulder

### Platform Match Implant

#### S implant

self-tapping, cylindrical implant  
with 0.8mm machined implant shoulder

### External Hex Implant

#### Mini implant

diameter-reduced, condensing, conical implant  
with 0.8mm machined implant shoulder

### Color coding/diameter

#### BEGO Semados® RS/RSX implant

3.0



#### BEGO Semados® Mini implant

2.7/2.9/3.1



#### BEGO Semados® S/SC/SCX implant

3.25



#### BEGO Semados® S/SC/SCX/RS/RSX/RI Implant

3.75



#### BEGO Semados® S/SC/SCX/RS/RSX/RI implant

4.1



#### BEGO Semados® S/SC/SCX/RS/RSX/RI implant

4.5




#### BEGO Semados® S/SC/SCX/RS/RSX/RI implant


5.5



# Label and sticker

- |        |   |   |
|--------|---|---|
| 1      |    | Manufacturer  |
| 2      |   | Article description/size information  |
| 3      |   | <b>Color coding</b><br> Ø 3.0  Ø 4.1<br> Ø 2.7 / 2.9 / 3.1  Ø 4.5<br> Ø 3.25  Ø 5.5<br> Ø 3.75 |
|        |    | <b>Article number</b>   |
|        |    | <b>Batch code</b>   |
|        |    | <b>Quantity</b>   |
|        |   | <b>Data Matrix Code</b><br>Includes manufacturer and article number.<br>If necessary, also batch number and/<br>or expiry date  |
| 4      |   | <b>Product description</b>  |
| 5      |    | <b>Use by</b>   |
|        |    | <b>CE marking</b>   |
|        |    | <b>Do not reuse</b>   |
|        |    | <b>Sterilized using irradiation</b>   |
|        |    | <b>Do not resterilize</b>   |
|        |    | <b>Non-sterile</b>  |
|        | <br>ifu.bego.com   | <b>Consult instructions for use<br/>for electronic instructions for use</b>   |
|        |    | <b>Do not use if package is damaged</b>   |
|        |    | <b>Caution</b>  |
|        |    | <b>Temperature limit</b>  |
|        |    | <b>Keep away from sunlight</b>  |
| RxOnly |   | According to US Federal law, this product may only be sold to trained physicians or on their behalf   |
|        |    | <b>Speed of rotation</b>  |
|        |    | <b>Packaging system comprising non-sterile protective packaging and a sterile barrier system</b>  |
|        |   | <b>Medical device</b>   |
|        |    | <b>MR conditional</b>   |
| 6      |    | <b>Product model</b>  |
|        |    | <b>Information website for patients</b>   |

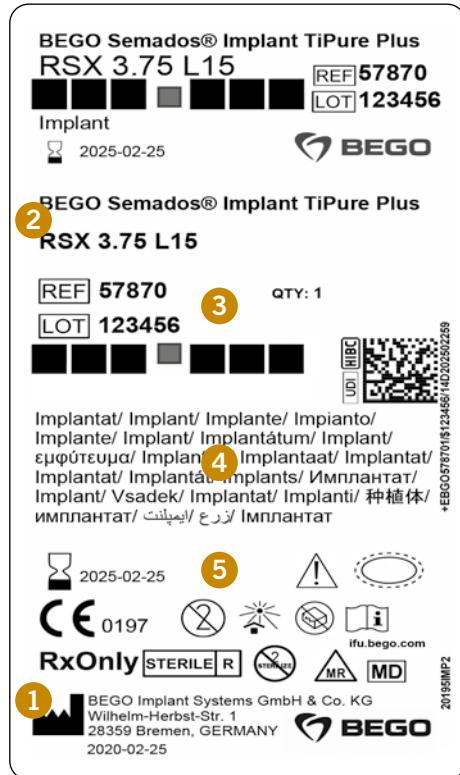

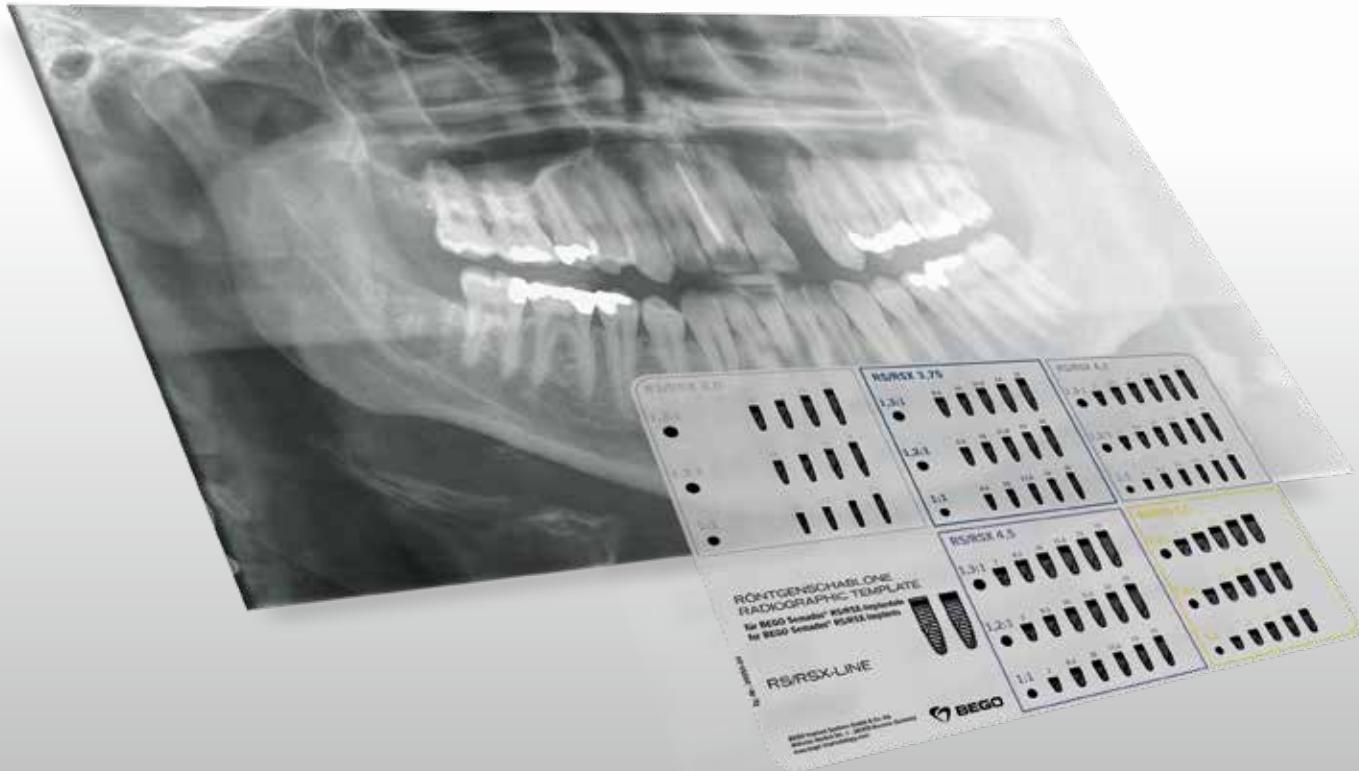

## OVERVIEW

Radiographic templates

20

Radiographic templates					
Description	REF	Color code	Size	Compatibility	Units
Radiographic templates	53888			S implants	1
	58246			SC/SCX implants	1
	57959			RS/RSX implants	1
	55745			RI implants	1
	57010			Mini implants	1
	57672			PI implants	1





## YOU HAVE THE CHOICE

### Your benefits

- SC/SCX implants – preservation of the crestal bone thanks to the integrated Platform Switch
- Efficient – just one surgical tray needed
- Well thought out – cover screw included
- Freedom of choice based on preference and indication – machined implant shoulder (SC implants) or micro-structured (SCX implants)
- Optional – Navigated/template-guided preparation of the BEGO Semados® SC/SCX implants with diameters 3.25–4.5 using the BEGO Guide system
- To satisfy the most stringent quality requirements – 100% German development and production

### Technical details

- Platform Switch
- Gap-free fit of the abutments thanks to the internal taper
- Self-tapping thread
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPurePlus surface
- Diameter: 3.25 · 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13 · 15mm
- Diameter 5.5mm in length 7mm if there is not much vertical bone height available



Consult instructions for use

## SURGERY · SC/SCX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion post TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	58160	■	3.25 L8.5	SC	1
	58161	■	3.25 L10	SC	1
	58162	■	3.25 L11.5	SC	1
	58163	■	3.25 L13	SC	1
	58164	■	3.25 L15	SC	1
	58165	■	3.75 L8.5	SC	1
	58166	■	3.75 L10	SC	1
	58167	■	3.75 L11.5	SC	1
	58168	■	3.75 L13	SC	1
	58169	■	3.75 L15	SC	1
	58170	■	4.1 L7	SC	1
	58171	■	4.1 L8.5	SC	1
	58172	■	4.1 L10	SC	1
	58173	■	4.1 L11.5	SC	1
	58174	■	4.1 L13	SC	1
	58175	■	4.1 L15	SC	1
	58176	■	4.5 L7	SC	1
	58177	■	4.5 L8.5	SC	1
	58178	■	4.5 L10	SC	1
	58179	■	4.5 L11.5	SC	1
	58180	■	4.5 L13	SC	1
	58181	■	4.5 L15	SC	1
	58182	■	5.5 L7	SC	1
	58183	■	5.5 L8.5	SC	1
	58184	■	5.5 L10	SC	1
	58185	■	5.5 L11.5	SC	1
	58186	■	5.5 L13	SC	1

**Note:** BEGO Semados® SC/SCX implants 3.25–4.5, template-guided preparation using the BEGO Guide System is an option.

<sup>\*5</sup> Platform Switch Design

## SURGERY · SC/SCX IMPLANTS WITH PS\*<sup>5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	58260	■	3.25 L8.5	SCX	1
	58261	■	3.25 L10	SCX	1
	58262	■	3.25 L11.5	SCX	1
	58263	■	3.25 L13	SCX	1
	58264	■	3.25 L15	SCX	1
	58265	■■	3.75 L8.5	SCX	1
	58266	■■	3.75 L10	SCX	1
	58267	■■	3.75 L11.5	SCX	1
	58268	■■	3.75 L13	SCX	1
	58269	■■	3.75 L15	SCX	1
	58270	■■	4.1 L7	SCX	1
	58271	■■	4.1 L8.5	SCX	1
	58272	■■	4.1 L10	SCX	1
	58273	■■	4.1 L11.5	SCX	1
	58274	■■	4.1 L13	SCX	1
	58275	■■	4.1 L15	SCX	1
	58276	■■■	4.5 L7	SCX	1
	58277	■■■	4.5 L8.5	SCX	1
	58278	■■■	4.5 L10	SCX	1
	58279	■■■	4.5 L11.5	SCX	1
	58280	■■■	4.5 L13	SCX	1
	58281	■■■	4.5 L15	SCX	1
	58282	■■■■	5.5 L7	SCX	1
	58283	■■■■	5.5 L8.5	SCX	1
	58284	■■■■	5.5 L10	SCX	1
	58285	■■■■	5.5 L11.5	SCX	1
	58286	■■■■	5.5 L13	SCX	1

Watch the video “BEGO Semados® SC/SCX implant”:




## SURGERY · SC/SCX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1



<sup>\*4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528  
<sup>\*5</sup> Platform Switch design

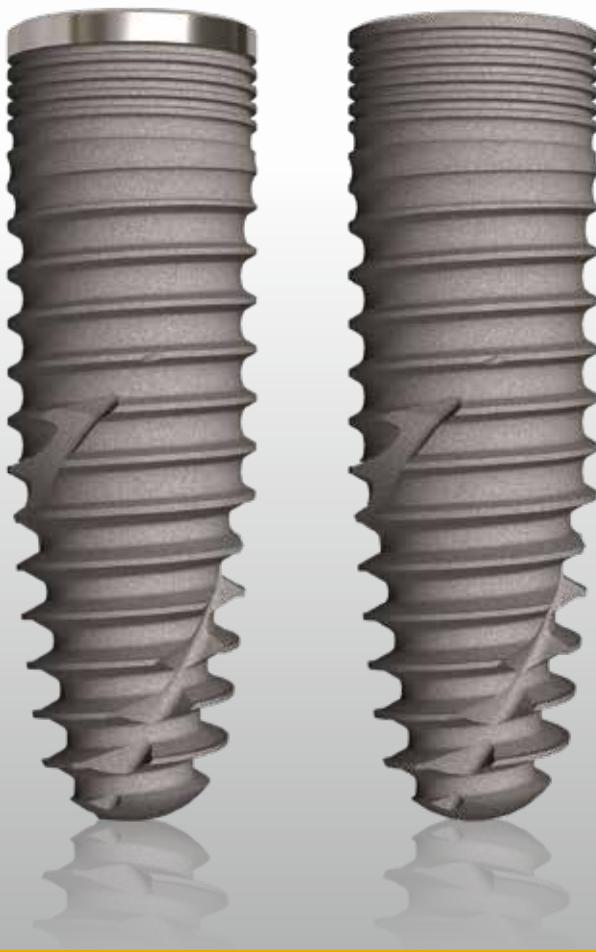

## FITS JUST ABOUT EVERY TIME

### Your benefits

- Simple to use – insert by self-centring
- Fast – only a few rotations needed for insertion
- Well thought out – cover screw included
- To satisfy the most stringent quality requirements – 100% German development and production
- Optional – Navigated/template-guided preparation of the BEGO Semados® RS/RSX implants with diameters 3.75–4.5 using the BEGO Guide system
- Established – conical inner connection with a mean conical angle of 45° and an internal hex that acts as an anti-rotation mechanism
- Integrated Platform Switch supports the preservation of the crestal bone

### Technical details

- Conical implant shape with rounded apex
- Self-tapping thread design with optimal cutting angle
- Diameter: 3.0 · 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13 · 15mm
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface
- Gap-free fit of the abutments thanks to the internal taper
- RS/RSX 3.0 suitable for use with narrow anterior gaps for the replacement of teeth 12, 22, 32–42
- Diameter 5.5 in length 7mm, for cases without appropriate vertical bone height available



Consult instructions for use

## SURGERY · RS/RSX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57962	□	3.0 L10	RS	1
	57963	□	3.0 L11.5	RS	1
	57964	□	3.0 L13	RS	1
	57966	■	3.75 L8.5	RS	1
	57967	■	3.75 L10	RS	1
	57968	■	3.75 L11.5	RS	1
	57969	■	3.75 L13	RS	1
	57970	■	3.75 L15	RS	1
	57971	■	4.1 L7	RS	1
	57972	■	4.1 L8.5	RS	1
	57973	■	4.1 L10	RS	1
	57974	■	4.1 L11.5	RS	1
	57975	■	4.1 L13	RS	1
	57976	■	4.1 L15	RS	1
	57977	■	4.5 L7	RS	1
	57978	■	4.5 L8.5	RS	1
	57979	■	4.5 L10	RS	1
	57980	■	4.5 L11.5	RS	1
	57981	■	4.5 L13	RS	1
	57982	■	4.5 L15	RS	1
	57983	■	5.5 L7	RS	1
	57984	■	5.5 L8.5	RS	1
	57985	■	5.5 L10	RS	1
	57986	■	5.5 L11.5	RS	1
	57987	■	5.5 L13	RS	1

**Note:** BEGO Semados® RS/RSX implants 3.0–4.5, template-guided preparation using the BEGO Guide System is an option.

<sup>\*5</sup> Platform Switch design

## SURGERY · RS/RSX IMPLANTS WITH PS\*<sup>5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57862	□	3.0 L10	RSX	1
	57863	□	3.0 L11.5	RSX	1
	57864	□	3.0 L13	RSX	1
	57866	■	3.75 L8.5	RSX	1
	57867	■	3.75 L10	RSX	1
	57868	■	3.75 L11.5	RSX	1
	57869	■	3.75 L13	RSX	1
	57870	■	3.75 L15	RSX	1
	57871	■	4.1 L7	RSX	1
	57872	■	4.1 L8.5	RSX	1
	57873	■	4.1 L10	RSX	1
	57874	■	4.1 L11.5	RSX	1
	57875	■	4.1 L13	RSX	1
	57876	■	4.1 L15	RSX	1
	57877	■	4.5 L7	RSX	1
	57878	■	4.5 L8.5	RSX	1
	57879	■	4.5 L10	RSX	1
	57880	■	4.5 L11.5	RSX	1
	57881	■	4.5 L13	RSX	1
	57882	■	4.5 L15	RSX	1
	57883	■	5.5 L7	RSX	1
	57884	■	5.5 L8.5	RSX	1
	57885	■	5.5 L10	RSX	1
	57886	■	5.5 L11.5	RSX	1
	57887	■	5.5 L13	RSX	1

Watch the video "BEGO Semados® RS/RSX implant":




## SURGERY · RS/RSX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1



<sup>\*4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528  
<sup>\*5</sup> Platform Switch design

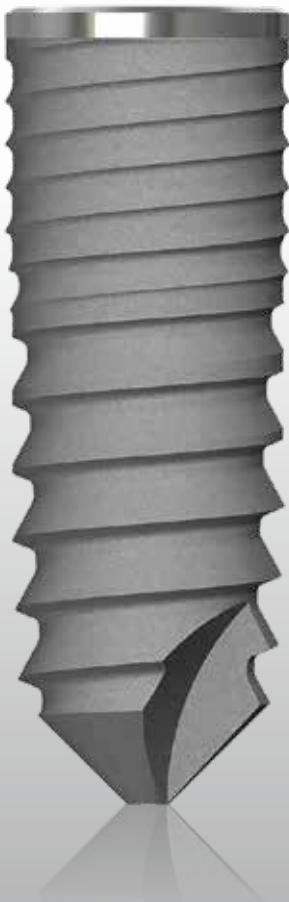

## CUTS A FINE FIGURE

### Your benefits

- Microthread in the neck region – for improved force transfer to the crestal bone
- Increase in the primary stability due to the condensing thread design for lateral bone compression
- Well thought out – cover screw included
- Integrated Platform Switch supports the preservation of the crestal bone
- To satisfy the most stringent quality requirements – 100% German development and production
- Stable connection with no micro-movements during functional masticatory loading (up to 150N)

### Technical details

- Self-condensing, conical implant with Platform Switch and 0.5mm machined implant shoulder
- Diameter: 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 8.5 · 10 · 11.5 · 13mm
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface
- Gap-free fit of the abutments thanks to the internal taper
- Internal hex prevents rotation of abutments



Consult instructions for use

## SURGERY · RI IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57708	■	3.75 L8.5	RI*1	1
	57709	■	3.75 L10	RI*1	1
	57710	■	3.75 L11.5	RI*1	1
	57711	■	3.75 L13	RI*1	1
	57718	■	4.1 L8.5	RI*1	1
	57719	■	4.1 L10	RI*1	1
	57720	■	4.1 L11.5	RI*1	1
	57721	■	4.1 L13	RI*1	1
	57728	■	4.5 L8.5	RI*1	1
	57729	■	4.5 L10	RI*1	1
	57730	■	4.5 L11.5	RI*1	1
	57731	■	4.5 L13	RI*1	1
	57738	■	5.5 L8.5	RI*1	1
	57739	■	5.5 L10	RI*1	1
	57740	■	5.5 L11.5	RI*1	1
	57741	■	5.5 L13	RI*1	1
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1

Watch the video "BEGO Semados® RI implant":



\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

\*4 Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 82528

\*5 Platform Switch design



## OVERVIEW

Cover screws	<b>32</b>
Healing abutments	<b>32</b>

## SURGERY · COVER SCREWS/HEALING ABUTMENTS WITH PS<sup>\*5</sup> DESIGN

Cover screws					
Description	REF	Color code	Size	Compatibility	Units
<b>Implant cover screws</b> Material: Titanium grade 4 (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57950	□		RS/RSX 3.0	1
	58290	■		SC/SCX 3.25	1
	57951	■■		SC/SCX/RS/RSX/RI <sup>*1</sup> 3.75	1
	57952	■■■		SC/SCX/RS/RSX/RI <sup>*1</sup> 4.1	1
	57953	■■■■		SC/SCX/RS/RSX/RI <sup>*1</sup> 4.5	1
	57954	■■■■■		SC/SCX/RS/RSX/RI <sup>*1</sup> 5.5	1

Healing abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS HP</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2					
<b>Implant diameter 3.0</b>					
	57764	□	Ø3.0 L3	RS/RSX 3.0	1
	57765	□	Ø3.0 L5	RS/RSX 3.0	1
	57766	□	Ø3.0 L7	RS/RSX 3.0	1
	57767	□	Ø4.0 L3	RS/RSX 3.0	1
	57768	□	Ø4.0 L5	RS/RSX 3.0	1
	57769	□	Ø4.0 L7	RS/RSX 3.0	1
<b>Implant diameter 3.25–3.75</b>					
	57807	■■	Ø4.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup> 3.25–3.75	1
	57808	■■	Ø4.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup> 3.25–3.75	1
	58150	■■	Ø4.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup> 3.25–3.75	1
<b>Implant diameter 4.1</b>					
	57809	■■	Ø5.0 L3	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.1	1
	57810	■■	Ø5.0 L5	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.1	1
	58151	■■	Ø5.0 L7	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.1	1
<b>Implant diameter 4.5</b>					
	57811	■■■	Ø5.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.5	1
	57812	■■■	Ø5.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.5	1
	58152	■■■	Ø5.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup> 4.5	1
<b>Implant diameter 5.5</b>					
	57813	■■■■	Ø6.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup> 5.5	1
	57814	■■■■	Ø6.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup> 5.5	1
	58153	■■■■	Ø6.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup> 5.5	1



\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

\*2 For torque specifications, see page 128

\*5 Platform Switch design

## SURGERY · COVER SCREWS/HEALING ABUTMENTS WITH PS<sup>\*5</sup> DESIGN

### Healing abutments

Description	REF	Color code	Size	Compatibility	Units
<b>PS HPW</b>					
prefabricated gingival former				<b>Implant diameter 3.25–3.75</b>	
Material: Titanium alloy	57815	■■	Ø 5.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
(packaged sterile)	58200	■■	Ø 5.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
Tool: Hexagon screwdriver	58201	■■	Ø 5.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
1.25mm/slot screwdriver				*2	
<b>Implant diameter 4.1</b>					
	57816	■	Ø 6.0 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
	58202	■	Ø 6.0 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
	58203	■	Ø 6.0 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
<b>Implant diameter 4.5</b>					
	57817	■	Ø 6.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
	58204	■	Ø 6.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
	58205	■	Ø 6.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
<b>Implant diameter 5.5</b>					
	57818	■	Ø 7.0 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	5.5
	58206	■	Ø 7.0 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	5.5




### Healing abutment

Description	REF	Color code	Size	Compatibility	Units
<b>Healing abutment, individual</b>					
customisable gingival former comprising:	55953	■■■■■	Ø 7.0	S/SC/SCX/RS/RSX/RI	3.25–5.5
• healing abutment					
• prosthesis screw Hex 1.25mm					
Material: Polyetheretherketone (PEEK)					
Tool: Hexagon screwdriver					
1.25mm					
*2					



---

<sup>\*7</sup> Platform Match design

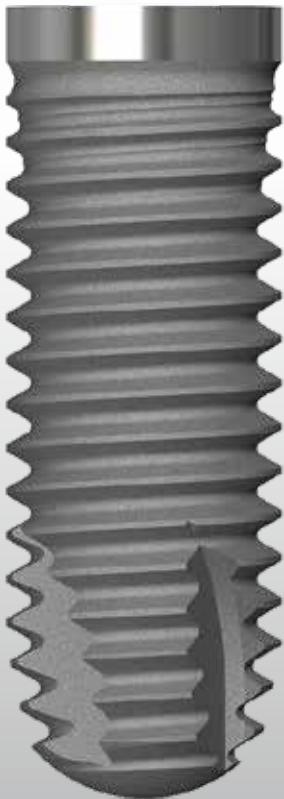

## YOUR TRIED-AND-TESTED SYSTEM – FAMILIAR YET NEW

### Your benefits

- S implants – increase in the primary stability thanks to increasing core diameter with decreasing thread depth
- Machined implant shoulder
- Well thought out – cover screw included
- Optional – Navigated/template-guided preparation of the BEGO Semados® S implants with diameters 3.25–4.5 using the BEGO Guide system
- To satisfy the most stringent quality requirements – 100% German development and production

### Technical details

- Platform Match
- Gap-free fit of the abutments thanks to the internal taper
- Self-tapping thread
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface
- Diameter: 3.25 · 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13mm



Consult instructions for use

SURGERY · IMPLANTS WITH PM<sup>®</sup> DESIGN

Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57500	■	3.25 L8.5	S	1
	57501	■	3.25 L10	S	1
	57502	■	3.25 L11.5	S	1
	57503	■	3.25 L13	S	1
	57601	■■	3.75 L8.5	S	1
	57602	■■	3.75 L10	S	1
	57603	■■	3.75 L11.5	S	1
	57604	■■	3.75 L13	S	1
	57840	■■■	4.1 L7	S	1
	57841	■■■	4.1 L8.5	S	1
	57842	■■■	4.1 L10	S	1
	57843	■■■	4.1 L11.5	S	1
	57844	■■■	4.1 L13	S	1
	57700	■■■■	4.5 L7	S	1
	57701	■■■■	4.5 L8.5	S	1
	57702	■■■■	4.5 L10	S	1
	57703	■■■■	4.5 L11.5	S	1
	57704	■■■■	4.5 L13	S	1
	57901	■■■■■	5.5 L8.5	S	1
	57902	■■■■■	5.5 L10	S	1
	57903	■■■■■	5.5 L11.5	S	1
	57904	■■■■■	5.5 L13	S	1
<b>BEGO SECURITY implants*<sup>4</sup></b>	83538				1
Implant warranty					

**Note:** BEGO Semados® S implants 3.25–4.5 mm template-guided preparation using the BEGO Guide System is an option.

<sup>a</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528.

\*<sup>7</sup> Platform Switch design



## OVERVIEW

Cover screws	<b>38</b>
Healing abutments	<b>38</b>

## SURGERY · COVER SCREWS/HEALING ABUTMENTS WITH PM\*<sup>7</sup> DESIGN

Cover screws					
Description	REF	Color code	Size	Compatibility	Units
<b>Implant cover screws</b> Material: Titanium grade 4 (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	55505	■		S 3.25	1
	55608	■		S/RI 3.75	1
	55615	■		S/RI 4.1	1
	55616	■		S/RI 4.5	1
	55908	■		S/RI 5.5	1


  

Healing abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Healing abutments</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2				<b>Healing abutment Ø 4.0</b>	
	55590	■ ■	L3	S/RI 3.25–3.75	1
	55591	■ ■	L5	S/RI 3.25–3.75	1
	55592	■ ■	L7	S/RI 3.25–3.75	1
				<b>Healing abutment Ø 4.5</b>	
	56300	■ ■ ■ ■	L3	S/RI 3.25–4.5	1
	56301	■ ■ ■ ■	L5	S/RI 3.25–4.5	1
	56302	■ ■ ■ ■	L7	S/RI 3.25–4.5	1
				<b>Healing abutment Ø 5.0</b>	
	55593	■ ■ ■ ■	L3	S/RI 3.25–4.5	1
	55594	■ ■ ■ ■	L5	S/RI 3.25–4.5	1
	55595	■ ■ ■ ■	L7	S/RI 3.25–4.5	1
				<b>Healing abutment Ø 6.0</b>	
	56303	■ ■ ■ ■ ■	L3	S/RI 3.25–5.5	1
	56304	■ ■ ■ ■ ■	L5	S/RI 3.25–5.5	1
	56305	■ ■ ■ ■ ■	L7	S/RI 3.25–5.5	1
<b>Healing abutment, conical</b> prefabricated gingival former for bar constructions Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2				<b>Healing abutments Ø 6.0</b>	
	57324	■ ■	L5	S/RI 3.25–3.75	1
<b>Healing abutment, individual</b> customisable gingival former comprising: • healing abutment • prosthesis screw Hex 1.25mm Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	55953	■ ■ ■ ■ ■	Ø 7.0	S/SC/SCX/RS/RSX/RI 3.25–5.5	1



\*2 For torque specifications, see p. 128

\*7 Platform Match design

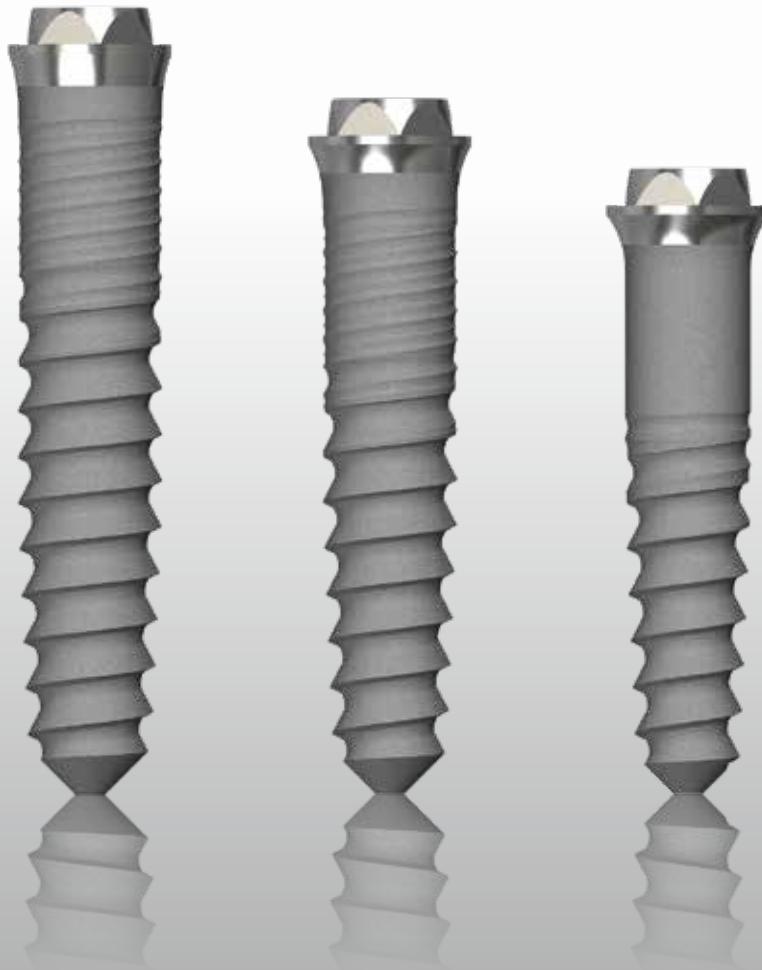

## MINI DONE DIFFERENTLY

### Your benefits

- Mini implants – an efficient implant system for narrow jaw restorations and narrow spaces
- Bionic design – avoids stress peaks in the implant and bone and increases the stability of the implants
- Well thought out – cover screw included
- To satisfy the most stringent quality requirements – 100% German development and production
- The laterally aligned thread flanks conform outstandingly well to the pre-shaped cavities
- Shortening of the treatment duration by avoiding elaborate augmentation procedures
- Correction of implant angulations thanks to conical external hex connection
- Large selection of prosthetic solutions available, including tension-free CAD/CAM-fabricated bar constructions
- Definitive restoration of edentulous, atrophied alveolar ridge with ready-to-use bar system

### Technical details

- Root-shaped, bone-condensing implant
- Diameter: 2.7 · 2.9 · 3.1mm
- Lengths: 11.5 · 13 · 15mm
- Single-tooth and ball attachment restoration possible with implant diameters 2.9mm and 3.1mm
- Easy-Con Mini restoration with implant diameter of 3.1mm
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface



Consult instructions for use

## SURGERY · MINI IMPLANTS/HEALING ABUTMENTS

Implants							
Description	REF	Color code	Size	Compatibility	Units		
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	56947	■ ■	2.7	L11.5	Mini	1	
	56948	■ ■	2.7	L13	Mini	1	
	56949	■ ■	2.7	L15	Mini	1	
	56950	■ ■	2.9	L11.5	Mini	1	
	56951	■ ■	2.9	L13	Mini	1	
	56952	■ ■	2.9	L15	Mini	1	
	56953	■ ■	3.1	L11.5	Mini	1	
	56954	■ ■	3.1	L13	Mini	1	
	56955	■ ■	3.1	L15	Mini	1	
<b>BEGO SECURITY implants*</b> <sup>4</sup>							
Implant warranty							



Cover screws						
Description	REF	Color code	Size	Compatibility	Units	
<b>Implant cover screws Mini</b> Material: Titanium grade 4 (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	56956	■	L2	Mini 2.7–3.1	1	

Healing abutments						
Description	REF	Color code	Size	Compatibility	Units	
<b>Healing abutments Mini</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hex wrench 1.25mm/slot screwdriver *2	56957	■	Ø3.5 L3	Mini 2.7–3.1	1	
	56958	■	Ø3.5 L4	Mini 2.7–3.1	1	
	57252	■	Ø3.5 L7	Mini 2.7–3.1	1	

Watch the video "BEGO Semados® Mini implant":



\*2 For torque specifications, see p. 128

\*4 Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528



## YOUR IMPLANT SYSTEM FOR A PROVISIONAL RESTORATION!

### Your benefits

- Best possible alignment – thanks to the malleable implant neck
- Narrow design – ideal if the available space is limited
- Prosthetic restoration – direct and indirect are options
- Universal use
- Relieves loads on augmented areas and the soft tissue
- Stabilizes bridges or dentures during the healing phase of the definitive implants
- For temporary restorations
- Fixation of templates for guided surgery
- Can be removed before insertion of the final restoration

### Technical details

- Diameter: 2.8mm
- Length: 14mm
- Fabricated from grade 5 titanium
- Untreated machined surface



Consult instructions for use

## SURGERY · PROVISIONAL IMPLANT SYSTEM

### Implants

Description	REF	Color code	Size	Compatibility	Units	
<b>BEGO Semados® Provisional Implant (PI)</b> Material: Titanium alloy (packaged sterile)	57660		Ø 2.8 L14		1	
	57673		Ø 2.8 L14		10	

### Surgical tray

Description	REF	Color code	Size	Compatibility	Units	
<b>BEGO Semados® PI Tray</b> incl. container, fully loaded	57670				1	
<b>BEGO Semados® PI Tray (empty)</b> empty tray, with container	58388				1	

### Impression taking

Description	REF	Color code	Size	Compatibility	Units	
<b>PI multifunctional cap</b> Material: Titanium alloy	57661				1	
	57674				5	

### Female parts

Description	REF	Color code	Size	Compatibility	Units	
<b>PI multifunctional cap</b> Material: Titanium alloy	57661				1	
	57674				5	
<b>PI protection cap</b> Material: Polyetheretherketone (PEEK) (packaged sterile)	57662				5	

### Implant analog

Description	REF	Color code	Size	Compatibility	Units	
<b>PI implant analog</b>	57671				1	

## SURGERY · PROVISIONAL IMPLANT SYSTEM

Instruments					
Description	REF	Color code	Size	Compatibility	Units
PI depth drill	57664		Ø 1.5 L20		1
					
PI paralleling post	57663				1
					
PI insert tool with W&H contra-angle connection	57665				1
					
BEGO Semados® ratchet adapter with ratchet connection for universal use of the ratchet (ratchet grips the adapter head/adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1
					
PI removal tool	57666				1
					
PI ratchet	57668				1
					
PI bending tool	57667				1
					
PI stabilizer	57669				1
					

Watch the video "BEGO Semados® Provisional Implant":







## OVERVIEW

BEGO Guide System S/SC/SCX implants

**46**

BEGO Guide System RS/RSX implants

**49**

## BEGO Guide System S/SC/SCX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide Tray</b> incl. container, fully loaded	57399			S/SC/SCX 3.25–4.5	1
					
Master sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide master sleeves</b>	57395		Ø 4.2 (A)	S/SC/SCX/RS/RSX	10
	57397		Ø 4.7 (B)	S/SC/SCX/RS/RSX	10
					
Reduction sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide spoons</b>	57411		Ø 1.6 (A1)	S/SC/SCX	1
	57412		Ø 2.5 (A2)	S/SC/SCX	1
	57413		Ø 2.8 (A3)	S/SC/SCX 3.25	1
	57414		Ø 3.25 (A4)	S/SC/SCX 3.75	1
	57415		Ø 1.6 (B1)	S/SC/SCX	1
	57416		Ø 2.5 (B2)	S/SC/SCX	1
	57417		Ø 2.8 (B3)	S/SC/SCX 3.25	1
	57418		Ø 3.25 (B4)	S/SC/SCX 3.75	1
	57419		Ø 3.65 (B5)	S/SC/SCX 4.1	1
	57420		Ø 4.0 (B6)	S/SC/SCX 4.5	1
					
Tissue punches					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide tissue punches</b>	57421		Ø 4.2 (A)	S/SC/SCX/RS/RSX 3.0–3.75	1
	57422		Ø 4.7 (B)	S/SC/SCX/RS/RSX 4.1–4.5	1
					

## BEGO Guide System S/SC/SCX implants

Preparation instruments						
Description	REF	Color code	Size	Compatibility	Units	
BEGO Guide centre drill	57459		Ø 4.2 (A)	S/SC/SCX/RS/RSX	3.0–3.75	1
	57463		Ø 4.7 (B)	S/SC/SCX/RS/RSX	4.1–4.5	1
BEGO Guide pilot drill	57423		Ø 1.6 L18 (X1)	S/SC/SCX		1
	57424		Ø 1.6 L23.5 (Y1)	S/SC/SCX		1
	57425		Ø 1.6 L29 (Z1)	S/SC/SCX		1
BEGO Guide depth drill	57426		Ø 2.5 L18 (X2)	S/SC/SCX		1
	57427		Ø 2.5 L23.5 (Y2)	S/SC/SCX		1
	57428		Ø 2.5 L29 (Z2)	S/SC/SCX		1
BEGO Guide depth drill	57429	■	Ø 2.8 L18 (X3)	S/SC/SCX	3.25	1
	57430	■	Ø 2.8 L23.5 (Y3)	S/SC/SCX	3.25	1
	57431	■	Ø 2.8 L29 (Z3)	S/SC/SCX	3.25	1
BEGO Guide depth drill	57432	■	Ø 3.25 L18 (X4)	S/SC/SCX	3.75	1
	57433	■	Ø 3.25 L23.5 (Y4)	S/SC/SCX	3.75	1
	57434	■	Ø 3.25 L29 (Z4)	S/SC/SCX	3.75	1
BEGO Guide depth drill	57435	■	Ø 3.65 L18 (X5)	S/SC/SCX	4.1	1
	57436	■	Ø 3.65 L23.5 (Y5)	S/SC/SCX	4.1	1
	57437	■	Ø 3.65 L29 (Z5)	S/SC/SCX	4.1	1
BEGO Guide depth drill	57438	■	Ø 4.0 L18 (X6)	S/SC/SCX	4.5	1
	57439	■	Ø 4.0 L23.5 (Y6)	S/SC/SCX	4.5	1
	57441	■	Ø 4.0 L29 (Z6)	S/SC/SCX	4.5	1
BEGO Guide countersink	57442	■	(3)	S/SC/SCX	3.25	1
	57443	■	(4)	S/SC/SCX	3.75	1
	57444	■	(5)	S/SC/SCX	4.1	1
	57445	■	(6)	S/SC/SCX	4.5	1

## BEGO Guide System S/SC/SCX implants

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide thread tap</b>	57446	■	(3)	S/SC/SCX 3.25	1
	57447	■	(4)	S/SC/SCX 3.75	1
	57448	■	(5)	S/SC/SCX 4.1	1
	57449	■	(6)	S/SC/SCX 4.5	1

Connector					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide connector</b>	57450		Ø 4.2 (AX)	S/SC/SCX	1
	57451		Ø 4.2 (AY)	S/SC/SCX	1
	57452		Ø 4.2 (AZ)	S/SC/SCX	1
	57453		Ø 4.7 (BX)	S/SC/SCX	1
	57454		Ø 4.7 (BY)	S/SC/SCX	1
	57455		Ø 4.7 (BZ)	S/SC/SCX	1

<b>BEGO Guide depth stop ring connector</b>	57456	Ø 4.2 (A)	S/SC/SCX/RS/RSX	1	
	57457	Ø 4.7 (B)	S/SC/SCX/RS/RSX	1	

<b>BEGO Guide ratchet adapter for connector</b>	57458		S/SC/SCX	1	
---	-------	--	----------	---	---

Watch video "BEGO Guide Tray (S/SC/SCX)":



## BEGO Guide System RS/RSX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide tray incl. container, fully loaded	58071			RS/RSX 3.0–4.5	1
BEGO Guide tray (empty) empty tray, with container	58386			RS/RSX 3.0–4.5	1
Master sleeves					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide master sleeves	57395		Ø 4.2 (A)	S/SC/SCX/RS/RSX	10
	57397		Ø 4.7 (B)	S/SC/SCX/RS/RSX	10
Reduction sleeves					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide Sp	57686		Ø 2.0 (A1)	RS/RSX	1
	57687		Ø 2.5 (A2)	RS/RSX	1
	57688		Ø 2.8 (A3)	RS/RSX 3.0	1
	57689		Ø 3.4 (A4)	RS/RSX 3.75	1
	57690		Ø 2.0 (B1)	RS/RSX	1
	57691		Ø 2.5 (B2)	RS/RSX	1
	57692		Ø 2.8 (B3)	RS/RSX 3.0	1
	57693		Ø 3.4 (B4)	RS/RSX 3.75	1
	57694		Ø 3.8 (B5)	RS/RSX 4.1	1
	57695		Ø 4.1 (B6)	RS/RSX 4.5	1
Tissue punches					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide tissue punches	57421	□ ■ ■	Ø 4.2 (A)	S/SC/SCX/RS/RSX 3.0–3.75	1
	57422	■ ■	Ø 4.7 (B)	S/SC/SCX/RS/RSX 4.1–4.5	1



## BEGO Guide System RS/RSX implants

Preparation instruments							
Description	REF	Color code	Size	Compatibility	Units		
<b>BEGO Guide centre drill</b> Pilot drill	57459		Ø 4.2 (A)	S/SC/SCX/RS/RSX	3.0–3.75	1	
	57463		Ø 4.7 (B)	S/SC/SCX/RS/RSX	4.1–4.5	1	
<b>BEGO Guide PD</b> Pilot drill	57696		Ø 2.0 L18 (X1)	RS/RSX	1		
	57697		Ø 2.0 L23.5 (Y1)	RS/RSX	1		
	57698		Ø 2.0 L29 (Z1)	RS/RSX	1		
<b>BEGO Guide DD</b> Depth drill	57713		Ø 2.5 L18 (X2)	RS/RSX	1		
	57714		Ø 2.5 L23.5 (Y2)	RS/RSX	1		
	57715		Ø 2.5 L29 (Z2)	RS/RSX	1		
<b>BEGO Guide DD</b> Depth drill	57716	□	Ø 2.8 L18 (X3)	RS/RSX	3.0	1	
	57717	□	Ø 2.8 L23.5 (Y3)	RS/RSX	3.0	1	
	57723	□	Ø 2.8 L29 (Z3)	RS/RSX	3.0	1	
<b>BEGO Guide DD</b> Depth drill	57724	■	Ø 3.4 L18 (X4)	RS/RSX	3.75	1	
	57725	■	Ø 3.4 L23.5 (Y4)	RS/RSX	3.75	1	
	57726	■	Ø 3.4 L29 (Z4)	RS/RSX	3.75	1	
<b>BEGO Guide DD</b> Depth drill	57727	■	Ø 3.8 L18 (X5)	RS/RSX	4.1	1	
	57733	■	Ø 3.8 L23.5 (Y5)	RS/RSX	4.1	1	
	57734	■	Ø 3.8 L29 (Z5)	RS/RSX	4.1	1	
<b>BEGO Guide DD</b> Depth drill	57735	■	Ø 4.1 L18 (X6)	RS/RSX	4.5	1	
	57736	■	Ø 4.1 L23.5 (Y6)	RS/RSX	4.5	1	
	57737	■	Ø 4.1 L29 (Z6)	RS/RSX	4.5	1	
<b>BEGO Guide CS</b> Countersink	58051	□	(3)	RS/RSX	3.0	1	
	58052	■	(4)	RS/RSX	3.75	1	
	58053	■	(5)	RS/RSX	4.1	1	
	58054	■	(6)	RS/RSX	4.5	1	

## BEGO Guide System RS/RSX implants

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide ST Thread tap</b>	58055	□	(3)	RS/RSX 3.0	1
	58056	■	(4)	RS/RSX 3.75	1
	58057	■	(5)	RS/RSX 4.1	1
	58058	■	(6)	RS/RSX 4.5	1

Connector					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide Conn with contra-angle connection</b>	58059		Ø 4.2 (AX)	RS/RSX	1
	58060		Ø 4.2 (AY)	RS/RSX	1
	58061		Ø 4.2 (AZ)	RS/RSX	1
	58062		Ø 4.7 (BX)	RS/RSX	1
	58063		Ø 4.7 (BY)	RS/RSX	1
	58064		Ø 4.7 (BZ)	RS/RSX	1

<b>BEGO Guide Conn with ratchet connection</b>	58065		Ø 4.2 (AX)	RS/RSX	1
	58066		Ø 4.2 (AY)	RS/RSX	1
	58067		Ø 4.2 (AZ)	RS/RSX	1
	58068		Ø 4.7 (BX)	RS/RSX	1
	58069		Ø 4.7 (BY)	RS/RSX	1
	58070		Ø 4.7 (BZ)	RS/RSX	1

<b>BEGO Guide depth stop ring connector</b>	57456		Ø 4.2 (A)	S/SC/SCX/RS/RSX	1
	57457		Ø 4.7 (B)	S/SC/SCX/RS/RSX	1

Watch video "BEGO Guide Tray (RS/RSX)":



## BEGO Guide System – Guided pilot drill holes

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide – pilot drill</b> for guided surgical pilot drill holes	57400		Ø 2.0 L22		1
	57401		Ø 2.0 L30		1



Drill sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide DS</b> for guided surgical pilot drill holes	57130		Ø 2.0		10





## OVERVIEW

BEGO Semados® S/SC/SCX implants	54
BEGO Semados® RS/RSX implants	57
BEGO Semados® RI implants	60
BEGO Semados® Mini implants	62
Surgical instruments	63
Bone shapers/trepans	64

## BEGO Semados® S/SC/SCX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Tray <sup>Plus</sup> incl. container, excl. drill module Ø 5.5 (REF 57347)	57340			S/SC/SCX 3.25–5.5	1
BEGO Semados® Tray <sup>Plus</sup> (empty) empty tray, with container	58351			S/SC/SCX 3.25–5.5	1
Drill module					
Description	REF	Color code	Size	Compatibility	Units
Drill module comprising: • depth drill, short • countersink • thread tap with ratchet connection	57347	■		S/SC/SCX 5.5	1
Reduced basic surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> incl. ratchet and container	58346			S/SC/SCX 3.75–4.5	1
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) empty tray, with container	58347			S/SC/SCX 3.75–4.5	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Pilot marker	57308		Ø 1.6 L15	S/SC/SCX	1
	57309		Ø 1.6 L23	S/SC/SCX	1

**BEGO Semados® S/SC/SCX implants**

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth drill 2.5	57100		Ø 2.5 L15	S/SC/SCX	1
	57101		Ø 2.5 L20	S/SC/SCX	1
Depth drill	57102	■	Ø 2.8 L15	S/SC/SCX 3.25	1
	57104	■	Ø 3.25 L15	S/SC/SCX 3.75	1
	57106	■	Ø 3.65 L15	S/SC/SCX 4.1	1
	57108	■	Ø 4.0 L15	S/SC/SCX 4.5	1
	57110	■	Ø 4.7 L15	S/SC/SCX 5.5	1
Depth drill	57103	■	Ø 2.8 L20	S/SC/SCX 3.25	1
	57105	■	Ø 3.25 L20	S/SC/SCX 3.75	1
	57107	■	Ø 3.65 L20	S/SC/SCX 4.1	1
	57109	■	Ø 4.0 L20	S/SC/SCX 4.5	1
Countersink	57350	■		S/SC/SCX 3.25	1
	57351	■		S/SC/SCX 3.75	1
	57352	■		S/SC/SCX 4.1	1
	57353	■		S/SC/SCX 4.5	1
	57354	■		S/SC/SCX 5.5	1
Thread tap	57332	■		S/SC/SCX 3.25	1
	57333	■		S/SC/SCX 3.75	1
	57334	■		S/SC/SCX 4.1	1
	57335	■		S/SC/SCX 4.5	1
	57336	■		S/SC/SCX 5.5	1

**BEGO Semados® S/SC/SCX implants**

Drill stop sets					
Description	REF	Color code	Size	Compatibility	Quantity
<b>Drill stops</b>	55804			Depth drill 2.5 and S/SC/SCX 3.25–3.75	1 set
	55715			S/SC/SCX 4.1	1 set
	55810			S/SC/SCX 4.5	1 set
	55910			S/SC/SCX 5.5	1 set
<b>Drill stop Tray<sup>Plus</sup></b> incl. storage box, lid and all drill stops	57345			S/SC/SCX	1 unit
<b>Drill stop Tray<sup>Plus</sup> (empty)</b> empty storage box, with lid	58354			S/SC/SCX	1 unit



## BEGO Semados® RS/RSX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Tray <sup>Plus</sup> incl. container, excl. drill module Ø 5.5 (REF 57948)	57949			RS/RSX 3.0-5.5	1
BEGO Semados® Tray <sup>Plus</sup> (empty) empty tray, with container	58350			RS/RSX 3.0-5.5	1
Drill module					
Description	REF	Color code	Size	Compatibility	Units
Drill module comprising: • depth drill, short • DD D1 (depth drill) • countersink • thread tap	57948	■		RS/RSX 5.5	1
Reduced basic surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> incl. ratchet and container	58348			RS/RSX 3.75-4.5	1
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) empty tray, with container	58349			RS/RSX 3.75-4.5	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Pilot marker	57481		Ø 1.6 L15	RS/RSX	1
	57482		Ø 1.6 L23	RS/RSX	1
Depth drill 2.5	57926		Ø 2.5 L15	RS/RSX	1
	57927		Ø 2.5 L20	RS/RSX	1



**BEGO Semados® RS/RSX implants**

Preparation instruments						
Description	REF	Color code	Size	Compatibility	Units	
Depth drill	57928	□	Ø 2.8 L15	RS/RSX	3.0	1
	57930	■	Ø 3.4 L15	RS/RSX	3.75	1
	57932	■	Ø 3.8 L15	RS/RSX	4.1	1
	57934	■	Ø 4.1 L15	RS/RSX	4.5	1
	57936	■	Ø 5.0 L15	RS/RSX	5.5	1
DD D1 (depth drill) In compact bone, particularly in the lower jaw, use depth drill DD D1 instead of the standard depth drill.	57484	□	Ø 2.9 L15	RS/RSX	3.0	1
	57485	■	Ø 3.6 L15	RS/RSX	3.75	1
	57486	■	Ø 4.0 L15	RS/RSX	4.1	1
	57487	■	Ø 4.3 L15	RS/RSX	4.5	1
	57488	■	Ø 5.3 L15	RS/RSX	5.5	1
Depth drill	57929	□	Ø 2.8 L20	RS/RSX	3.0	1
	57931	■	Ø 3.4 L20	RS/RSX	3.75	1
	57933	■	Ø 3.8 L20	RS/RSX	4.1	1
	57935	■	Ø 4.1 L20	RS/RSX	4.5	1
Countersink	57937	□		RS/RSX	3.0	1
	57938	■		RS/RSX	3.75	1
	57939	■		RS/RSX	4.1	1
	57940	■		RS/RSX	4.5	1
	57941	■		RS/RSX	5.5	1
Thread tap	57943	□		RS/RSX	3.0	1
	57944	■		RS/RSX	3.75	1
	57945	■		RS/RSX	4.1	1
	57946	■		RS/RSX	4.5	1
	57947	■		RS/RSX	5.5	1

**BEGO Semados® RS/RSX implants**

Drill stop sets					
Description	REF	Color code	Size	Compatibility	Quantity
Drill stops	57476		Depth drill 2.5	RS/RSX	1 set
	57477	□		RS/RSX 3.0	1 set
	57478	■		RS/RSX 3.75	1 set
	57479	■■		RS/RSX 4.1–4.5	1 set
	57480	■■■		RS/RSX 5.5	1 set
Drill stop Tray <sup>Plus</sup> incl. storage box, lid and all drill stops	57483			RS/RSX	1 unit
Drill stop Tray <sup>Plus</sup> (empty) empty storage box, with lid	58356			RS/RSX	1 unit



## BEGO Semados® RI implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Tray <sup>Plus</sup> incl. container, excl. drill module Ø 5.5 (REF 57613)	57612			RI 3.75–5.5	1
BEGO Semados® Tray <sup>Plus</sup> (empty) empty tray, with container	58352			RI 3.75–5.5	1
Drill module					
Description	REF	Color code	Size	Compatibility	Units
Drill module comprising: • depth drill • countersink • threadformer • screw tap	57613	■		RI 5.5	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Pilot marker	57581		Ø 2.5 L16	RI	1
	57582		Ø 2.5 L25	RI	1
Depth drill 3.2	57583		Ø 3.2 L15	RI	1
	57584		Ø 3.2 L20	RI	1

**BEGO Semados® RI implants**

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth drill	57585	■	Ø 3.52 L15	RI 3.75	1
	57587	■	Ø 3.93 L15	RI 4.1	1
	57589	■	Ø 4.32 L15	RI 4.5	1
	57591	■	Ø 5.28 L15	RI 5.5	1
Depth drill	57586	■	Ø 3.52 L20	RI 3.75	1
	57588	■	Ø 3.93 L20	RI 4.1	1
	57590	■	Ø 4.32 L20	RI 4.5	1
Countersink	57592	■		RI 3.75	1
	57593	■		RI 4.1	1
	57594	■		RI 4.5	1
	57595	■		RI 5.5	1
Threadformer	55766	■		RI 3.25	1
	57615	■		RI 3.75	1
	57616	■		RI 4.1	1
	57617	■		RI 4.5	1
	57618	■		RI 5.5	1
Thread tap	57619	■		RI 3.75	1
	57620	■		RI 4.1	1
	57621	■		RI 4.5	1
	57622	■		RI 5.5	1

**BEGO Semados® Mini implants**

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
Mini/Osseoplus Tray incl. container, fully loaded	56970			Mini 2.7–3.1	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Initial drill	55714				1
DD (depth drill)	57995	■ ■	Ø 2.55 L16.5	Mini 2.7	1
	57996	■ ■	Ø 2.75 L16.5	Mini 2.9	1
	57997	■ ■	Ø 2.95 L16.5	Mini 3.1	1
Threadformer	56979	■ ■		Mini 2.7	1
	56980	■ ■		Mini 2.9	1
	56981	■ ■		Mini 3.1	1

## Surgical instruments

Surgical instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>Drill extension, one-part without internal cooling</b>	57265			Extension of 15.8mm	1
<b>Insert tool for implants with ratchet connection</b>	55831		L6		1
	55830		L12.5		1
<b>Insert tool for implants with contra-angle connection</b>	56990		L21.5		1
	55832		L24		1
<b>IDC (adjustment instrument) for making final corrections to the position of the inserted implant after removal of the insertion post</b>	56749	□		RS/RSX 3.0	1
	56748			S/SC/SCX/RS/RSX/RI 3.25–5.5	1
<b>Guiding wrench spanner and guide pin for tools with ratchet connection</b>	53897				1
<b>Paralleling post</b>	55863			S/SC/SCX	2
	57956			RS/RSX	2
	57598			RI	1
	56972			Mini	1

## Surgical instruments

Surgical instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth gauge	53872			S/SC/SCX	1
	55746			RI	1
	57955			RS/RSX	1
Ratchet/ torque wrench for torques 10–50Ncm	55799				1
BEGO Semados® ratchet adapter with ratchet connection for uni- versal use of the ratchet (ratchet grips the adapter head/adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1

## Bone shapers/trepans

Bone shapers					
Description	REF	Color code	Size	Compatibility	Units
PS BP	58445	□		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.0	1
	58446	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58447	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58448	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58449	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1

## Trepan drill

Trepan drill					
Description	REF	Color code	Size	Compatibility	Units
Trepan drill	55817		Ø 4.2 external/Ø 3.7 internal	L20	1
	55815		Ø 5.0 external/Ø 4.1 internal	L20	1
	56991		Ø 5.0 external/Ø 4.3 internal	L20	1
	55816		Ø 6.0 external/Ø 5.1 internal	L20	1

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design



## OVERVIEW

Instruments	<b>66</b>
CAD/CAM Implant Prosthetics BEGO Medical	<b>67</b>
Prosthetics SC/SCX/RS/RSX/RI <sup>*1</sup> implants (Platform Switch design)	<b>75</b>
Prosthetics S implants (Platform Match design)	<b>97</b>
Prosthetics Mini implants	<b>115</b>

## PROSTHETICS · INSTRUMENTS



Prosthetic tray					
Description	REF	Color code	Size	Compatibility	Units
<b>Prosthetic kit</b> with ratchet/torque wrench, hexagon screwdriver 1.25mm short/long, slot screwdriver long, insert tool for ball attachment, insert tool 3Locator®, ratchet adapter, incl. storage box and lid	55826				1
<b>Prosthetic kit (empty)</b> empty storage box, with lid	58357				1
Prosthetic instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>Hexagon screwdriver</b> <b>1.25mm</b> with conical ratchet connection for implant cover screws, healing abutments, impression posts, insertion posts and prosthe- sis screws	57266		L5		1
	53949		L10		1
	53948		L17		1
<b>Hexagon screwdriver</b> <b>1.25mm contra-angle</b> conical for implant cover screws, healing abutments, impression posts, insertion posts and Prosthesis screws	55563		L25		1
	55564		L31		1
<b>Slot screwdriver</b> with ratchet connection For technician screws, healing abutments and impression posts	53952		L14		1
<b>Ratchet/torque wrench</b> for torques 10–50Ncm	55799				1
<b>BEGO Semados®</b> <b>ratchet adapter</b> with ratchet connection for uni- versal use of the ratchet (ratchet grips the adapter head /adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1

**Note:** Manufacturer notes about trade names, see page 125.



## OVERVIEW

Interface overview	68
Individual healing abutments	69
Individual abutments	69
Occlusal screw-retained bridge restorations	71
Bar constructions	72

Interface overview								
Implant diameter	Platform	Color code	CADAbut Full	CADAbut Duo with anti-rotation protection	CADAbut Duo without anti-rotation protection	CADBase implant level	CADBase abutment level	
			 	     	   	 		
<b>BEGO Implant Systems – Semados® SC/SCX/RS/RSX/RI implants – Platform Switch design</b>								
RS/RSX 3.0	3.0	□						
SC/SCX 3.25	3.67	■						
SC/SCX/RS/RSX/RI 3.75	3.67	■	✓					
SC/SCX/RS/RSX/RI 4.1	4.1	■		✓				
SC/SCX/RS/RSX/RI 4.5	4.5	■				✓	✓	✓
SC/SCX/RS/RSX/RI 5.5	5.5	■						
<b>BEGO Implant Systems – Semados® S implants – Platform Match design</b>								
3.25	3.67	■						
3.75	3.67	■						
4.1	4.1	■	✓			✓	✓	✓
4.5	4.5	■			✓			
5.5	5.5	■						
<b>BEGO Implant Systems – Semados® MultiPlus</b>								
3.25; 3.75; 4.1; 4.5; 5.5	Abutment level							✓
<b>BEGO Implant Systems – Semados® Mini implants (exclusively for bars)</b>								
2.7; 2.9; 3.1	3.5	■					✓	

## Individual healing abutments – patient-specific soft tissue management for outstanding aesthetics

### BEGO CADAbut Full – one-part individual healing abutments incl. prosthesis screw

Description	Units	
BEGO titanium grade 5 only for temporary use	1	

### BEGO CADAbut Duo – two-part individual healing abutments (plus titanium adhesive abutment)

Description	Units	
BEGO PMMA Multicolor available in 3 shades (M01, M02, M03), only for temporary use	1	

## Individual abutments – one- and two-part abutments

### BEGO CADAbut Full – one-part individual abutments incl. prosthesis screw

Description	Units	
Wirobond® MI+	1	
BEGO titanium grade 5	1	
Extras Fully anatomical shape	1	

<b>BEGO CADAbut Duo – two-part individual healing abutments (plus titanium adhesive abutment)</b>		
Description	Compatibility	Units
<b>BEGO Zirkon LT</b> available in 5 shades (LT01–LT05)		1
		
<b>KATANA<sup>®</sup> Zirconia STML</b> available in 13 VITA <sup>®</sup> classical shades.		1
		
<b>IPS e.max<sup>®</sup> CAD</b> Delivered in blue pre-crystallized state. LT can be supplied in the 16 VITA <sup>®</sup> classical shades. MO can be supplied in five opaque shades.	SC/SCX/RS/RSX/RI <sup>†</sup>	1
		
<b>CAD/Cast<sup>®</sup> alloys</b> Selected BEGO precious metal alloys at the currently valid daily price; request the current prices. (Tel. +49 421 20 28-251)		1
		
<b>Wirobond<sup>®</sup> C+</b>		1
		
<b>BEGO PMMA Multicolor</b> available in 3 shades (M01, M02, M03), only for temporary use		1
		

<sup>†</sup> Only for BEGO Semados<sup>®</sup> implants with Platform Switch design.<sup>®</sup>This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

## Occlusal screw-retained one- and two-part bridge restorations

### BEGO CADBase implant level/abutment level – one-part individual bridge constructions incl. prosthesis screw

Description	Product description	Units
<b>BEGO titanium grade 5</b>	Occlusal screw-retained bridge/framework	2–4
	Occlusal screw-retained bridge/framework	5–7
	Occlusal screw-retained bridge/framework	≥ 8
	Angled screw channel 0°–20°	
	Pontic/bridge member	
<b>Wirobond® M+</b>	Occlusal screw-retained bridge/framework	2–4
	Occlusal screw-retained bridge/framework	5–7
	Occlusal screw-retained bridge/framework	≥ 8
	Angled screw channel 0°–20°	
	Pontic/bridge member	



### DYNAMIC ABUTMENT®

Description	REF	Units
<b>Screwdriver L24</b> for prosthesis screw angled screw channels	549539	1



### BEGO CADAbut Duo without anti-rotation protection – two-part individual bridge constructions (plus titanium adhesive abutment)

Description	Product description	Units
<b>BEGO Zirkon LT</b> Bridge constructions for partial and full veneers with up to 16 units and up to two bridge members, available in five shades (LT01–LT05)	Occlusal screw-retained bridge/framework	up to 16
	Pontic/bridge member	up to 2
<b>KATANA®<sup>6</sup> Zirconia STML</b> up to three units, available in 13 VITA <sup>®</sup> classical shades	Occlusal screw-retained bridge/framework	up to 3
	Pontic/bridge member	up to 1
<b>BEGO PMMA Multicolor</b> Only for temporary bridge restorations With up to 16 units and one pontic, available in three shades (M01, M02, M03).	Occlusal screw-retained bridge/framework	up to 16
	Pontic/bridge member	up to 1
<b>Wirobond® C+</b> Bridge constructions for partial and full veneers with up to 16 units and up to four bridge members	Occlusal screw-retained bridge/framework	up to 4
	Pontic/bridge member	≥ 4
	Pontic/bridge member	> 4
Fully anatomical bridge construction with up to 16 units and up to four bridge members	Occlusal screw-retained bridge/framework	up to 4
	Pontic/bridge member	≥ 4
	Pontic/bridge member	> 4



## Bar constructions – milled bars and bar bases made from titanium or cobalt-chromium

BEGO CADBase (bar bases incl. prosthesis screws)		
Description	Number of implant units	
BEGO titanium grade 5	2–4	
	5–7	
	≥8	
Wirobond® Mi+	2–4	
	5–7	
	≥8	

BEGO CADBar		
Description	Units	
BEGO titanium grade 5	1	
Wirobond® Mi+	1	

Bar joint attachments		
Description	Cross-section	
Round bar 1.8mm		
Horix® <sup>6</sup> bar 1.8mm		
Dolder® <sup>6</sup> bar joint attachment 2.3mm		
Dolder® <sup>6</sup> bar joint attachment 3.0mm		

**Indication:** Implant/mucosa-supported removable prosthesis on at least two implants (without extensions)

**Note:** Bridge constructions not available for BEGO Semados® RS/RSX implants Ø3.0 and Mini implants!

<sup>6</sup>This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

**Bar attachments****Description**

Dolder<sup>\*6</sup> bar attachments  
3.0mm

**Cross-section**

**Individual bar shapes/  
bar attachments**



**Indication:** Implant-supported removable prosthesis on at least four implants (with extensions)

**Additional retention elements****Description****Units****Bar attachments****available for:**

- Ancora<sup>\*6</sup>/Preci-Vertix<sup>\*6</sup> 1.8mm
- Preci-Vertix<sup>\*6</sup> Crown
- Preci-Vertix<sup>\*6</sup> Bar

1



**Thread drills for retention  
elements,**

1

**available for:**

- Zest Anchors<sup>\*6</sup>
- CEKA<sup>\*6</sup> attachment M2
- CEKA<sup>\*6</sup> attachment M3
- CEKA<sup>\*6</sup> ball anchor M2

**Drill elements**

1.9–3.0mm

1

**Bar element**Preci-Horix<sup>\*6</sup> 1.8mm

1

**Retention elements****Description**

Dolder<sup>\*6</sup> bar female parts  
**palladium alloy**  
Resilience bar attachments,  
female parts with retention  
for polymer



available from  
Ceka-Vertrieb Deutschland,  
Akazienstraße 7A, 30169 Hanover,  
Germany  
Tel. +49 511 8070041,  
[www.cka-vertrieb.de](http://www.cka-vertrieb.de)

**Ancora female parts (Preci-Vertix rider/Preci-Horix<sup>\*6</sup> rider)**

Description	REF	Size	Units
<b>Ancora</b> Universal rider rigid	52593	Ø 1.8mm	1
Also available from BEGO Bremer Goldschlägerei Wilh. Herbst GmbH & Co. KG, Wilhelm-Herbst-Str. 1, 28359 Bremen, Germany, Tel. +49 421 2028-0, Fax +49 421 2028-100, email: info@bego.com, www.bego.com			

**Bar secondary structure**

Description	Units
<b>Wirobond® C+</b> including pin, hole, and/or bead retentions	1
<b>Hybrid with Wirobond® C+</b> including pin, hole and/or bead retentions	i



For questions about individually fabricated CAD/CAM implant prosthetics from BEGO Medical GmbH (procedure or conditions), please contact:

BEGO Medical GmbH  
Wilhelm-Herbst-Str. 1 · 28359 Bremen,  
Germany

Tel. +49 421 2028-0 · Fax +49 421 2028-174  
email info@bego-medical.de · www.bego.com

**Note:** Bridge constructions not available for BEGO Semados® RS/RSX implants Ø 3.0 and Mini implants!

<sup>\*1</sup> New version of the BEGO Semados® RI implant, with Platform Switch design

<sup>\*5</sup> Platform Switch design

<sup>\*6</sup> This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.



## OVERVIEW

CAD/CAM restoration	<b>76</b>
One Care Package restoration	<b>79</b>
Impression taking and model fabrication	<b>80</b>
Crown restoration Ø 3.0	<b>81</b>
Crown and bridge restoration	<b>82</b>
Multi <sup>Plus</sup> restoration	<b>88</b>
Hybrid restoration	<b>92</b>
Screws	<b>95</b>

**Note:** The entire Platform Switch prosthetics range is **not** compatible with the previous S/RI implants (with the Platform Match design)! For these implants, please only use the structures/components listed from page 97 onward.

**CAD/CAM restoration Ø 3.0**

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CADP</b> comprising: • PS CAD positioner • PScrew Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58250	□		RS/RSX 3.0	1



Adhesive abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB</b> comprising: • PS adhesive abutment • PScrew • TScrew Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57781	□		RS/RSX 3.0	1



**Note:** When using the \*<sup>6</sup>Cerec® system, a \*<sup>6</sup>InLab scanbody for \*<sup>6</sup>Bluecam (36 units) REF 6431303 or a scanbody for \*<sup>6</sup>Omnicam (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

## CAD/CAM restoration Ø 3.25–5.5

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CADP</b> comprising: <ul style="list-style-type: none"><li>• PS CAD positioner</li><li>• prosthesis screw Hex 1.25mm</li></ul> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58251	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58252	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58253	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58254	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1

Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB</b> comprising: <ul style="list-style-type: none"><li>• PS adhesive abutment Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57823	■■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58370	■■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57824	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58371	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57825	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58372	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57826	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58373	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1

Scansupports					
Description	REF	Color code	Size	Compatibility	Units
<b>CAD SP</b> comprising: <ul style="list-style-type: none"><li>• scansupport</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58191	■■		S/SC/SCX/RS/RSX/RI 3.25–3.75	1
	58192	■		S/SC/SCX/RS/RSX/RI 4.1	1
	58193	■		S/SC/SCX/RS/RSX/RI 4.5	1
	58194	■		S/SC/SCX/RS/RSX/RI 5.5	1

Options for downloading adhesive geometries for decentralized fabrication are available online at [www.bego.com](http://www.bego.com)



## CAD/CAM restoration Ø 3.25–5.5

Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB NH</b> comprising: <ul style="list-style-type: none"><li>• PS adhesive abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57827		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58374		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57828		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58375		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57829		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58376		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57830		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58377		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Milling blank					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PMB</b> comprising: <ul style="list-style-type: none"><li>• milling blank</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58326		Ø 11.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1
	58226		Ø 16	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1



Ti-Form milling blank					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PMB</b> comprising: <ul style="list-style-type: none"><li>• milling blank Ti-Form</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li><li>• AmannGirrbach Intellicode</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58221			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1



ceramill® CAD/CAM

**Note:** For the PS PMB (milling blank) a \*<sup>6</sup>PreFace abutment holder for the corresponding milling system is required. This must be ordered directly from the machine manufacturer. Please note the manufacturer's information regarding this!

**Note:** PS PMB (Ti-Form milling blank), Original System Partner from ceramill CAD/CAM

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

## One Care Package restoration

Restoration sets					
Description	REF	Color code	Size	Compatibility	Units
<b>PS OCP</b> comprising: <ul style="list-style-type: none"><li>• OCP abutment</li><li>• multifunctional cap</li><li>• impression coping</li><li>• laboratory cap for crowns</li><li>• laboratory cap for bridges</li><li>• prosthesis screw Sub-Tec<sup>plus</sup></li></ul> Material: Titanium alloy/ polyetheretherketone (PEEK)/ polycarbonate (PC) (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	58297		GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58300		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58298		GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58301		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58299		GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58302		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1

Laboratory caps for crowns					
Description	REF	Color code	Size	Compatibility	Units
<b>LCC</b> Material: Polycarbonate (PC)	58303				5

Laboratory caps for bridges					
Description	REF	Color code	Size	Compatibility	Units
<b>LCB</b> Material: Polycarbonate (PC)	58304				5

Implant analog					
Description	REF	Color code	Size	Compatibility	Units
<b>OCP A</b> Material: Titanium alloy	58305				1

Watch the video "BEGO Semados® One Care Package – OCP":



## Impression taking and model fabrication Ø 3.0–5.5

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CTI</b> Impression taking on implant with closed tray comprising: <ul style="list-style-type: none"><li>• impression post cap</li><li>• PS impression post</li><li>• titanium screw</li></ul> Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57773	□		RS/RSX 3.0	1
	58316	■		SC/SCX 3.25	1
	57799	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57800	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57801	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57802	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS OTI</b> Impression taking on implant with open tray comprising: <ul style="list-style-type: none"><li>• PS impression post</li><li>• titanium screw short/long</li></ul> Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57774	□		RS/RSX 3.0	1
	58317	■		SC/SCX 3.25	1
	57803	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57804	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57805	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57806	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>PS IMPA</b>	57796	□		RS/RSX 3.0	1
	58315	■		SC/SCX 3.25	1
	57819	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57820	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57821	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57822	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



* <sup>4</sup> DIM-Analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BPS 5.DIM</b>	549320	□		RS/RSX 3.0	1
	549321	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	549322	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	549323	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	549324	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

## Crown restoration Ø 3.0

Provisional					
Description	REF	Color code	Size	Compatibility	Units
<b>PS ITA</b> Material: Titanium alloy Tool: Insert tool for implants *2	57778	<input type="checkbox"/>		RS/RSX 3.0	1




Solid abutments, titanium					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiAA</b> angle over plane (type P) or edge (type E) comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• PScrew</li><li>• TScrew</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57797	<input type="checkbox"/>	15° P GH 2.5–4	RS/RSX 3.0	1
	57798	<input type="checkbox"/>	15° E GH 2.5–4	RS/RSX 3.0	1
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• PScrew</li><li>• TScrew</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57776	<input type="checkbox"/>	GH 2.5–4	RS/RSX 3.0	1



Angulated abutment, type P	Angulated abutment, type E
Type P = angle over plane	Type E = angle over edge



## Crown and bridge restoration Ø 3.25–5.5

Temporary abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PPA</b> Solid abutment, plastic for provisional restorations comprising: <ul style="list-style-type: none"><li>• PS plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	58072	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58073	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58074	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58075	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
					
<b>PS TPA</b> comprising: <ul style="list-style-type: none"><li>• PS plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	58146	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58147	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58148	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
					
<b>PS TTiA</b> comprising: <ul style="list-style-type: none"><li>• provisional PS titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57854	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57855	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57856	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57857	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
					
<b>PS TTiA NH</b> comprising: <ul style="list-style-type: none"><li>• provisional PS titanium abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57858	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57859	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57860	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57861	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
					
<b>PS ITA</b> Material: Titanium alloy Tool: Insert tool Implants * <sup>2</sup>	58076	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58077	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58078	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
					

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design\*<sup>2</sup> For torque specifications, see page 128\*<sup>5</sup> Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment, conical</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58088			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58089			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58090			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58091			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57846		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57847		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57848		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57849		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57850		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57851		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57852		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	57853		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



## Crown and bridge restoration Ø 3.25–5.5

Solid abutments						
Description	REF	Color code	Size	Compatibility	Units	
<b>PS TiAA</b> angle over plane (type P) or edge (type E) comprising: • PS titanium abutment • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57889	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57890	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57891	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57892	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57893	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57894	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57895	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57896	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57897	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57898	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57899	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57900	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57905	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57906	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57907	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57908	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design\*<sup>2</sup> For torque specifications, see page 128\*<sup>5</sup> Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

Solid abutments						
Description	REF	Color code	Size	Compatibility	Units	
PS TiAA angle over plane (type P) or edge (type E) comprising: • PS titanium abutment • prosthesis screw Sub-Tec <sup>plus</sup> • technician screw Sub-Tec <sup>plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57909	■■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57910	■■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57911	■■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57912	■■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75	1
	57913	■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57914	■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57915	■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57916	■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1	1
	57917	■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57918	■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57919	■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57920	■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5	1
	57921	■■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57922	■■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57923	■■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1
	57924	■■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5	1



Angulated abutment, type P	Angulated abutment, type E
Type P = angle over plane	Type E = angle over edge



Selection set					
Description	REF	Color code	Size	Compatibility	Units
PS AS For selecting the correct abutment with corresponding gingival height and angle, comprising: • 20 parts + forceps	58247		0°/15°/20°	SC/SCX/RS/RSX/RI* <sup>1</sup>	1



## Crown and bridge restoration Ø 3.25–5.5

Universal abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS UNI</b> comprising: <ul style="list-style-type: none"><li>• PS universal base Hex</li><li>• wax-up sleeve Universal</li><li>• PS UNI PScrew</li><li>• PS UNI TScrew (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57831			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57832			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57833			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57834			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS UNI NH</b> comprising: <ul style="list-style-type: none"><li>• PS universal base no Hex</li><li>• wax-up sleeve Universal</li><li>• PS UNI PScrew</li><li>• PS UNI TScrew (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57835			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57836			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57837			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57838			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>Internal reamer Universal</b> For re-working the internal form fit	55536			S/SC/SCX/RS/RSX/RI 3.25–5.5	1
<b>External reamer Universal</b> For re-working the external form fit	55537			S/SC/SCX/RS/RSX/RI 3.25–5.5	1

Watch the video “BEGO Semados® Universal Abutment”:



Watch the video “BEGO Semados® Universal Abutment no Hex”:



\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>3</sup> Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

\*<sup>5</sup> Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

### Gold cast-on abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>PS GCO</b> comprising: <ul style="list-style-type: none"><li>• PS cast-on abutment</li><li>• wax-up sleeve for gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	58092	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1	
	58093	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1	
	58094	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1	
<b>PS GCO NH</b> comprising: <ul style="list-style-type: none"><li>• PS cast-on abutment no Hex</li><li>• wax-up sleeve for gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	58096	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1	
	58097	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1	
	58098	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1	
	58099	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1	
<b>Internal reamer for gold cast-on abutment</b> For re-working the internal form fit (a technician screwdriver is recommended as the hold)	53735	■■■■■		S/SC/SCX/RS/RSX/RI 3.25–5.5	1	

## MultiPlus restoration

Auxiliary parts					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus insertion splint</b> To determine the planned angle	57532			MultiPlus System	1
<b>MultiPlus alignment aids</b> For aligning the implant hex	57530	20°		MultiPlus System	1
	57531	30°		MultiPlus System	1

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS MultiPlus</b> comprising: • PS abutment 0° • MultiPlus positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument MultiPlus abutment 0° * <sup>2</sup>	58100	■■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	58101	■■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	58102	■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	58103	■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	58104	■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	58105	■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
<b>Insertion instrument MultiPlus</b> <b>abutment 0°</b> with ratchet connection	57533			MultiPlus System	1

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design\*<sup>2</sup> For torque specifications, see page 128\*<sup>5</sup> Platform Switch design

## Multi<sup>Plus</sup> restoration

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS Multi<sup>Plus</sup></b> comprising: • PS Multi <sup>Plus</sup> abutment 20° • Multi <sup>Plus</sup> positioning aid 20° • prosthesis screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	58108	■■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58109	■■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58110	■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58111	■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58112	■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58113	■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
<b>PS Multi<sup>Plus</sup></b> comprising: • PS Multi <sup>Plus</sup> abutment 30° • Multi <sup>Plus</sup> positioning aid 30° • prosthesis screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	58116	■■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58117	■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58118	■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
Healing posts					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> healing post</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57520		L5	Multi <sup>Plus</sup> System	1
<b>Multi<sup>Plus</sup> healing post</b> <b>Mushroom</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57521		L5	Multi <sup>Plus</sup> System	1



## Multi<sup>Plus</sup> restoration

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> closed-tray impression</b> impression taking on Multi <sup>Plus</sup> abutments on closed trays comprising: <ul style="list-style-type: none"><li>• Multi<sup>Plus</sup> impression posts</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57522		L8	Multi <sup>Plus</sup> System	1
	57554		L12	Multi <sup>Plus</sup> System	1
					
<b>Multi<sup>Plus</sup> open-tray impression</b> impression taking on Multi <sup>Plus</sup> abutments on open trays comprising: <ul style="list-style-type: none"><li>• Multi<sup>Plus</sup> impression posts</li><li>• titanium screws L11 and L16</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57523		L8	Multi <sup>Plus</sup> System	1
					

Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> implant analogs</b>	57524			Multi <sup>Plus</sup> System	1
	57525			Multi <sup>Plus</sup> System	4
					

<sup>4</sup> DIM analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG MU 5.DIM</b>	549528			Multi <sup>Plus</sup> System	1
					

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

## Multi<sup>Plus</sup> restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>CADP Multi<sup>Plus</sup></b> • CAD positioner Multi <sup>Plus</sup> • secondary screw Multi <sup>Plus</sup> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58255			Multi <sup>Plus</sup> System	1
					
Titanium abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> titanium abutment</b> comprising: • Multi <sup>Plus</sup> titanium abutment • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57526		L11	Multi <sup>Plus</sup> System	1
					
Universal abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> Universal</b> comprising: • Multi <sup>Plus</sup> wax-up sleeve Universal • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2	57538		L11	Multi <sup>Plus</sup> System	1
					
<b>Internal reamer Multi<sup>Plus</sup></b> For re-working the internal form fit, incl. reamer handle	57540			Multi <sup>Plus</sup> System	1
					
<b>External reamer Multi<sup>Plus</sup></b> For re-working the external form fit, incl. reamer handle	57539			Multi <sup>Plus</sup> System	1
					

Watch the video "BEGO Semados® Multi<sup>Plus</sup> System":



**Crown restoration Ø 3.75–5.5**

Easy-Con abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS Easy-Con</b> Material: Titanium alloy with TiN coating Tool: Insert tool <sup>3</sup> Locator® * <sup>2</sup>	58130	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58131	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58132	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58133	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58134	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58135	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58136	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58137	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58138	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58139	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58140	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58141	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58142	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58143	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>Insert tool Easy-Con/ <sup>3</sup>Locator® with ratchet connection</b>	57008				1



Easy-Con impression taking					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con impression coping</b> Impression on Easy-Con	57751				4
<b>Easy-Con analog</b>	57760				4



**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

## Crown restoration Ø 3.75–5.5

Easy-Con female parts					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con laboratory set comprising:</b> <ul style="list-style-type: none"><li>• retention insert transparent, pink and blue</li><li>• block-out ring</li><li>• retention cap</li><li>• production insert, black</li></ul> Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
<b>Easy-Con instrument</b> For screw-fitting, removing, and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
<b>Easy-Con production insert (black)</b> Material: Polyamide (PA12)	57754				4
<b>Easy-Con retention insert (blue)</b> Withdrawal force approx.: 917g; 9N; 0°–10°   Material: Polyamide (PA12)	57755				4
<b>Easy-Con retention insert (pink)</b> Withdrawal force approx.: 1427g; 14N; 0°–10°   Material: Polyamide (PA12)	57756				4
<b>Easy-Con retention insert (transparent)</b> Withdrawal force approx.: 2243g; 22N; 0°–10°   Material: Polyamide (PA12)	57757				4
<b>Easy-Con retention insert (red)</b> Withdrawal force approx.: 663g; 6.5N; 10°–20°   Material: Polyamide (PA12)	57758				4
<b>Easy-Con retention insert (green)</b> Withdrawal force approx.: 2599g; 25.5N; 10°–20°   Material: Polyamide (PA12)	57759				4

Watch the video “BEGO Semados® Easy-Con System (chairside)”: <https://www.youtube.com/watch?v=JyfjwvzDQIY>



Watch the video “BEGO Semados® Easy-Con System (laboratory)”: <https://www.youtube.com/watch?v=JyfjwvzDQIY>



## Crown restoration Ø 3.25–4.5

Ball attachment abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS BA</b> comprising: <ul style="list-style-type: none"><li>• PS ball attachment without female parts</li><li>• spacer</li></ul> Material: Titanium alloy Tool: Insert tool Ball attachment <sup>*2</sup>	58120		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58121		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58122		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58123		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58124		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58125		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58126		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58127		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58128		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
Insert tool for ball attachment with ratchet connection					
	55880				1
Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment impression set <sup>2</sup>Dalbo®-PLUS</b> impression on ball attachment comprising: <ul style="list-style-type: none"><li>• impression post cap for ball attachment (red)</li><li>• implant analog for ball attachment</li></ul>	55768				1
Ball attachment female parts <sup>2</sup> Dalbo®					
Description	REF	Color code	Size	Compatibility	Units
<b>Female parts <sup>2</sup>Dalbo®-PLUS</b> comprising: <ul style="list-style-type: none"><li>• female parts <sup>2</sup>Dalbo®-PLUS, complete (incl. retention insert)</li><li>• placeholder</li></ul> Material: Titanium grade 4 Tool: <sup>2</sup> Dalbo®-PLUS activator/de-activator	55769				1
<b>Activator/Deactivator <sup>2</sup>Dalbo®-PLUS</b>	55773				1
<b>Retention insert <sup>2</sup>Dalbo®-PLUS</b> Material: Precious metal Tool: <sup>2</sup> Dalbo®-PLUS activator/de-activator	55776				1

Watch the video "BEGO Semados® Ball Attachment":



## Screws

Prosthesis screws					
Description	REF	Color code	Size	Compatibility	Units
Prosthesis screw Hex 1.25mm	53999			Healing abutments, individual Ø 7, PS CADP, PS PPA, PS TPA, PS GCO/PS GCO NH	1
Prosthesis screw Sub-Tec <sup>Plus</sup>	57031			CAD SP, PS CATI, PS OCP, PS PMB, PS TiB/PS TiB NH, PS TTiA/PS TTiA NH, PS TiAA, PS TiA	1
Secondary screw Multi <sup>Plus</sup> (M1.4)	57534			Multi <sup>Plus</sup> System	1
Prosthesis screw Multi <sup>Plus</sup> (M1.8)	57535			PS Multi <sup>Plus</sup> 20°/30°	1
PScrew	57782	<input type="checkbox"/>		Prosthesis Ø 3.0	1
PScrew	57784	<input type="checkbox"/>		CAD positioner Ø 3.0	1
PS UNI PScrew	57993			PS UNI/PS UNI NH	1

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 128

\*<sup>5</sup> Platform Switch design

---

<sup>\*7</sup> Platform Match design



## OVERVIEW

CAD/CAM restoration	98
Impression taking and model fabrication	100
Crown and bridge restoration	101
Multi <sup>Plus</sup> restoration	106
Hybrid restoration	110
Screws	113

## CAD/CAM restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec CAD positioner</b> comprising: • Sub-Tec CAD positioner • prosthesis screw Hex 1.25mm Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	57060			S/RI 3.25–5.5	1



Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec CAD/CAM titanium adhesive abutment</b> comprising: • Sub-Tec adhesive abutment • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57285			S/RI 3.25–3.75	1
	57287			S/RI 4.1	1
	57289			S/RI 4.5	1
	57291			S/RI 5.5	1
<b>Sub-Tec CAD/CAM titanium adhesive abutment no Hex</b> comprising: • Sub-Tec adhesive abutment no Hex • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57286			S/RI 3.25–3.75	1
	57288			S/RI 4.1	1
	57290			S/RI 4.5	1
	57292			S/RI 5.5	1



\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

\*2 For torque specifications, see page 128

\*6 This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

\*7 Platform Match design

## CAD/CAM restoration

### Adhesive abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>Sub-Tec CAD/CAM TiBase L</b> comprising:	57656	■■		S/RI 3.25–3.75	1	
• Sub-Tec TiBase	57657	■		S/RI 4.1	1	
• prosthesis screw Sub-Tec <sup>Plus</sup>	57658	■		S/RI 4.5	1	
• technician screw Sub-Tec <sup>Plus</sup>	57659	■		S/RI 5.5	1	
Material: Titanium alloy						
Tool: Hexagon screwdriver 1.25mm						
*2						



### Scansupport

Description	REF	Color code	Size	Compatibility	Units	
<b>CAD SP</b> comprising:	58191	■■		S/SC/SCX/RS/RSX/RI 3.25–3.75	1	
• scansupport	58192	■		S/SC/SCX/RS/RSX/RI 4.1	1	
• prosthesis screw Sub-Tec <sup>Plus</sup>	58193	■		S/SC/SCX/RS/RSX/RI 4.5	1	
Material: Titanium alloy	58194	■		S/SC/SCX/RS/RSX/RI 5.5	1	
Tool: Hexagon screwdriver 1.25mm						
*2						



### Milling blanks

Description	REF	Color code	Size	Compatibility	Units	
<b>ST PMB</b> comprising:	58319	■■■■■	Ø 11.5	S/RI 3.25–5.5	1	
• milling blank	58219	■■■■■	Ø 16	S/RI 3.25–5.5	1	
• prosthesis screw Sub-Tec <sup>Plus</sup>						
• technician screw Sub-Tec <sup>Plus</sup>						
Material: Titanium alloy						
Tool: Hexagon screwdriver 1.25mm						
*2						



**Note:** When using the \*<sup>6</sup>Cerec® system, a \*<sup>6</sup>Cerec / \*<sup>6</sup>InLab scanbody for \*<sup>6</sup>Bluecam (36 units) REF 6431303 or a scanbody for \*<sup>6</sup>Omnicam (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

**Note:** For the ST PMB a \*<sup>6</sup>PreFace® abutment holder for the corresponding milling system is required. This must be ordered directly from the machine manufacturer. Please note the manufacturer's information regarding this!

## Impression taking and model fabrication

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Dent closed-tray impression</b> Impression taking on implant with closed tray comprising: <ul style="list-style-type: none"><li>• impression post cap</li><li>• sub impression posts</li><li>• titanium screw L11</li></ul> Tool: Hexagon screwdriver 1.25mm *2	55860	■		S 3.25	1
	55539	■		S/RI 3.75	1
	55617	■		S/RI 4.1	1
	55618	■		S/RI 4.5	1
	55551	■		S/RI 5.5	1
					
<b>Sub-Dent open-tray impression</b> Impression taking on implant with open tray comprising: <ul style="list-style-type: none"><li>• sub impression posts</li><li>• titanium screws L16 and L21</li></ul> Tool: Hexagon screwdriver 1.25mm *2	55861	■		S 3.25	1
	55540	■		S/RI 3.75	1
	55619	■		S/RI 4.1	1
	55620	■		S/RI 4.5	1
	56500	■		S/RI 5.5	1
					

Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>Model implants</b>	56694	■		S 3.25	1
	56695	■		S/RI 3.75	1
	56696	■		S/RI 4.1	1
	56698	■		S/RI 4.5	1
	56699	■		S/RI 5.5	1
					

<sup>4</sup> DIM analogs <sup>®</sup>					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG 5.DIM</b>	549316	■■		S/RI 3.25–3.75	1
	549317	■		S/RI 4.1	1
	549318	■		S/RI 4.5	1
	549319	■		S/RI 5.5	1
					

**Note:** Manufacturer notes about trade names, see page 125.

\*2 For torque specifications, see p. 128

<sup>\*7</sup> Platform Match design

## Crown and bridge restoration

Provisional abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec provisional abutment</b> solid abutment, plastic for provisional restorations comprising: <ul style="list-style-type: none"><li>• plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	55951		Ø7	S/RI 3.25–5.5	1
<b>Sub-Tec provisional PEEK abutment</b> comprising: <ul style="list-style-type: none"><li>• plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	57494			S/RI 3.25–3.75	1
	57495			S/RI 4.1–4.5	1
<b>Sub-Tec provisional titanium abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec provisional titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57304			S/RI 3.25–3.75	1
	57305			S/RI 4.1	1
	57306			S/RI 4.5	1
	57307			S/RI 5.5	1
<b>Sub-Tec provisional titanium abutment no Hex</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec provisional titanium abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57300			S/RI 3.25–3.75	1
	57301			S/RI 4.1	1
	57302			S/RI 4.5	1
	57303			S/RI 5.5	1



## Crown and bridge restoration

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec<sup>Plus</sup> titanium abutment comprising:</b>	57116		GH 1–2	S/RI 3.25–3.75	1
• titanium abutment	57117		GH 2.5–4	S/RI 3.25–3.75	1
• prosthesis screw Sub-Tec <sup>Plus</sup>	57120		GH 1–2	S/RI 4.1	1
• technician screw Sub-Tec <sup>Plus</sup>	57121		GH 2.5–4	S/RI 4.1	1
Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57124		GH 1–2	S/RI 4.5	1
	57125		GH 2.5–4	S/RI 4.5	1
	57128		GH 1–2	S/RI 5.5	1
	57129		GH 2.5–4	S/RI 5.5	1



\*2 For torque specifications, see p. 128  
\*7 Platform Match design

## Crown and bridge restoration

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec<sup>Plus</sup> titanium angulated abutment</b> angle over plane (type P) or edge (type E) comprising: <ul style="list-style-type: none"><li>• angulated abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57132		15° P GH 1–2	S/RI 3.25–3.75	1
	57133		15° P GH 2.5–4	S/RI 3.25–3.75	1
	57134		15° E GH 1–2	S/RI 3.25–3.75	1
	57135		15° E GH 2.5–4	S/RI 3.25–3.75	1
	57136		15° P GH 1–2	S/RI 4.1	1
	57137		15° P GH 2.5–4	S/RI 4.1	1
	57138		15° E GH 1–2	S/RI 4.1	1
	57139		15° E GH 2.5–4	S/RI 4.1	1
	57140		15° P GH 1–2	S/RI 4.5	1
	57141		15° P GH 2.5–4	S/RI 4.5	1
	57142		15° E GH 1–2	S/RI 4.5	1
	57143		15° E GH 2.5–4	S/RI 4.5	1
	57144		15° P GH 1–2	S/RI 5.5	1
	57145		15° P GH 2.5–4	S/RI 5.5	1
	57146		15° E GH 1–2	S/RI 5.5	1
	57147		15° E GH 2.5–4	S/RI 5.5	1



### Angulated abutment, type P

Type P = angle over plane



### Angulated abutment, type E

Type E = angle over edge



## Crown and bridge restoration

Universal abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec Universal</b> comprising: <ul style="list-style-type: none"><li>• Universal base Hex</li><li>• sub wax-up sleeve Universal</li><li>• prosthesis screw Sub-Tec Universal</li><li>• technician screw Sub-Tec Universal (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	55525			S/RI 3.25–3.75	1
	55622			S/RI 4.1	1
	55527			S/RI 4.5	1
	55529			S/RI 5.5	1
<b>Sub-Tec Universal no Hex</b> comprising: <ul style="list-style-type: none"><li>• Universal base no Hex</li><li>• sub wax-up sleeve Universal</li><li>• prosthesis screw Sub-Tec Universal</li><li>• technician screw Sub-Tec Universal (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	55526			S/RI 3.25–3.75	1
	55623			S/RI 4.1	1
	55528			S/RI 4.5	1
	55530			S/RI 5.5	1
<b>Internal reamer Universal</b> For re-working the internal form fit	55536			S/SC/SCX/RS/RSX/RI	3.25–5.5
<b>External reamer Universal</b> For re-working the external form fit	55537			S/SC/SCX/RS/RSX/RI	3.25–5.5

Watch the video “BEGO Semados® Universal Abutment”:



Watch the video “BEGO Semados® Universal Abutment no Hex”:



\*2 For torque specifications, see p. 128

\*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

\*7 Platform Match design

## Crown and bridge restoration

### Gold cast-on abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>Sub-Tec gold cast-on</b> comprising:	55862	■■		S/RI 3.25–3.75	1	
• sub cast-on abutment	55624	■		S/RI 4.1	1	
• sub wax-up sleeve gold cast-on	56317	■		S/RI 4.5	1	
• prosthesis screw Hex 1.25mm						
• technician screw						
Material: Gold/platinum alloy						
Tool: Hexagon screwdriver						
1.25mm						
*2 *3						
<b>Sub-Tec gold cast-on no Hex</b> comprising:	55873	■■		S/RI 3.25–3.75	1	
• sub cast-on abutment no Hex	55625	■		S/RI 4.1	1	
• sub wax-up sleeve gold cast-on	56325	■		S/RI 4.5	1	
• prosthesis screw Hex 1.25mm	56515	■		S/RI 5.5	1	
• technician screw						
Material: Gold/platinum alloy						
Tool: Hexagon screwdriver						
1.25mm						
*2 *3						
<b>Internal reamer for gold cast-on abutment</b> For re-working the internal form fit (a technician screwdriver is recommended as the hold)	53735	■■■■■		S/SC/SCX/RS/RSX/RI	3.25–5.5	

## MultiPlus restoration

Auxiliary parts					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus insertion splint</b> To determine the planned angle	57532			MultiPlus System	1
<b>MultiPlus alignment aids</b> For aligning the implant hex	57530		20°	MultiPlus System	1
	57531		30°	MultiPlus System	1

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec MultiPlus abutments</b> comprising: • Sub-Tec MultiPlus abutment 0° • MultiPlus positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument MultiPlus abutment 0° *2	57505	■■	0° GH 1	S/RI 3.25–3.75	1
	57508	■■	0° GH 3	S/RI 3.25–3.75	1
	57506	■	0° GH 1	S/RI 4.1	1
	57509	■	0° GH 3	S/RI 4.1	1
	57507	■	0° GH 1	S/RI 4.5	1
	57510	■	0° GH 3	S/RI 4.5	1
<b>Insertion instrument</b> <b>MultiPlus abutment 0°</b> with ratchet connection	57533			MultiPlus System	1

\*2 For torque specifications, see p. 128  
\*7 Platform Match design

## Multi<sup>Plus</sup> restoration

### Abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>Sub-Tec Multi<sup>Plus</sup> abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec Multi<sup>Plus</sup> abutment 20°</li><li>• Multi<sup>Plus</sup> positioning aid 20°</li><li>• prosthesis screw Multi<sup>Plus</sup></li></ul> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57511		20° GH 2.3–0.6	S/RI 3.25–3.75	1	
	57514		20° GH 4.0–2.3	S/RI 3.25–3.75	1	
	57512		20° GH 2.3–0.6	S/RI 4.1	1	
	57515		20° GH 4.0–2.3	S/RI 4.1	1	
	57513		20° GH 2.3–0.6	S/RI 4.5	1	
	57516		20° GH 4.0–2.3	S/RI 4.5	1	
<b>Sub-Tec Multi<sup>Plus</sup> abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec Multi<sup>Plus</sup> abutment 30°</li><li>• Multi<sup>Plus</sup> positioning aid 30°</li><li>• prosthesis screw Multi<sup>Plus</sup></li></ul> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57517		30° GH 4.0–1.5	S/RI 3.25–3.75	1	
	57518		30° GH 4.0–1.5	S/RI 4.1	1	
	57519		30° GH 4.0–1.5	S/RI 4.5	1	



### Healing posts

Description	REF	Color code	Size	Compatibility	Units	
<b>Multi<sup>Plus</sup> healing post</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57520		L5	Multi <sup>Plus</sup> System	1	
<b>Multi<sup>Plus</sup> healing post</b> <b>Mushroom</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57521		L5	Multi <sup>Plus</sup> System	1	



## MultiPlus restoration

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus closed-tray impression</b> impression taking on MultiPlus abutments on closed trays comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57522		L8	MultiPlus System	1
	57554		L12	MultiPlus System	1
					
<b>MultiPlus open-tray impression</b> (impression taking on MultiPlus abutments on open trays) comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li><li>• titanium screws L11 and L16</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57523		L8	MultiPlus System	1
					
Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus implant analogs</b>	57524			MultiPlus System	1
	57525			MultiPlus System	4
					
<sup>4</sup> DIM-Analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG MU 5.DIM</b>	549528			MultiPlus System	1
					

**Note:** Manufacturer notes about trade names, see page 125.

\*2 For torque specifications, see p. 128

\*7 Platform Match design

## Multi<sup>Plus</sup> restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>CADP Multi<sup>Plus</sup></b> • CAD positioner Multi <sup>Plus</sup> • secondary screw Multi <sup>Plus</sup> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58255			Multi <sup>Plus</sup> System	1
					
Titanium abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> titanium abutment</b> comprising: • Multi <sup>Plus</sup> titanium abutment • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57526		L11	Multi <sup>Plus</sup> System	1
					
Universal abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> Universal</b> comprising: • Multi <sup>Plus</sup> wax-up sleeve Universal • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25mm	57538		L11	Multi <sup>Plus</sup> System	1
					
<b>Internal reamer Multi<sup>Plus</sup></b> For re-working the internal form fit, incl. reamer handle	57540			Multi <sup>Plus</sup> System	1
					
<b>External reamer Multi<sup>Plus</sup></b> For re-working the external form fit, incl. reamer handle	57539			Multi <sup>Plus</sup> System	1
					

Watch the video "BEGO Semados® Multi<sup>Plus</sup> System":



## Hybrid restoration

Easy-Con abutments					
Description	REF	Color code	Size	Compatibility	Units
Sub-Tec Easy-Con abutment Material: Titanium alloy with TiN coating Tool: Insert tool <sup>3</sup> Locator® *2	57743	■■	L1	S/RI 3.75–4.1	1
	57744	■■	L2	S/RI 3.75–4.1	1
	57745	■■	L3	S/RI 3.75–4.1	1
	57746	■■	L4	S/RI 3.75–4.1	1
	57747	■	L1	S/RI 4.5	1
	57748	■	L2	S/RI 4.5	1
	57749	■	L3	S/RI 4.5	1
	57750	■	L4	S/RI 4.5	1
Insert tool Easy-Con/ <sup>3</sup> Locator® with ratchet connection	57008				1



Easy-Con impression taking					
Description	REF	Color code	Size	Compatibility	Units
Easy-Con impression coping Impression on Easy-Con	57751				4
Easy-Con analog	57760				4



**Note:** Manufacturer notes about trade names, see page 125.

\*2 For torque specifications, see p. 128

\*7 Platform Match design

## Hybrid restoration

### Easy-Con female parts

Description	REF	Color code	Size	Compatibility	Units	
<b>Easy-Con laboratory set comprising:</b> <ul style="list-style-type: none"><li>• retention insert transparent, pink, and blue</li><li>• block-out ring</li><li>• retention cap</li><li>• production insert, black</li></ul> Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2	
<b>Easy-Con instrument</b> For screw-fitting, removing, and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1	
<b>Easy-Con production insert (black)</b> Material: Polyamide (PA12)	57754				4	
<b>Easy-Con retention insert (blue)</b> Withdrawal force approx.: 917g; 9N; 0–10°   Material: Polyamide (PA12)	57755				4	
<b>Easy-Con retention insert (pink)</b> Withdrawal force approx.: 1427g; 14N; 0–10°   Material: Polyamide (PA12)	57756				4	
<b>Easy-Con retention insert (transparent)</b> Withdrawal force approx.: 2243g; 22N; 0–10°   Material: Polyamide (PA12)	57757				4	
<b>Easy-Con retention insert (red)</b> Withdrawal force approx.: 663g; 6.5N; 10–20°   Material: Polyamide (PA12)	57758				4	
<b>Easy-Con retention insert (green)</b> Withdrawal force approx.: 2599g; 25.5N; 10–20°   Material: Polyamide (PA12)	57759				4	

Watch the video "BEGO Semados® Easy-Con System (chairside)":



Watch the video "BEGO Semados® Easy-Con System (laboratory)":



## Hybrid restoration

Ball attachment abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec ball attachment comprising:</b>	57631		GH 0	S/RI 3.25–3.75	1
• sub ball attachment without female parts	57633		GH 3	S/RI 3.25–3.75	1
• spacer	57635		GH 5	S/RI 3.25–3.75	1
Material: Titanium alloy	57632		GH 0	S/RI 4.1–4.5	1
Tool: Insert tool	57634		GH 3	S/RI 4.1–4.5	1
Ball attachment	57636		GH 5	S/RI 4.1–4.5	1
<sup>*2</sup>					
<b>Insert tool for ball attachment with ratchet connection</b>	55880				1



Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment impression set <sup>2</sup>Dalbo®-PLUS</b>	55768				1
impression on ball attachment comprising:					
• impression post cap for ball attachment (red)					
• implant analog for ball attachment					



Ball attachment female parts <sup>2</sup> Dalbo®					
Description	REF	Color code	Size	Compatibility	Units
<b>Female parts <sup>2</sup>Dalbo®-PLUS</b>	55769				1
comprising:					
• female parts <sup>2</sup> Dalbo®-PLUS, complete (incl. retention insert)					
• placeholder					
Material: Titanium grade 4					
Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator					
<b><sup>2</sup>Dalbo®-PLUS activator/deactivator</b>	55773				1
<b>Retention insert <sup>2</sup>Dalbo®-PLUS</b>	55776				1
Material: Precious metal					
Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator					



Watch the video “BEGO Semados® Ball Attachment”:



<sup>\*7</sup> Platform Match design

## Screws

Prosthesis screws					
Description	REF	Color code	Size	Compatibility	Units
Prosthesis screw Hex 1.25mm	53999			Sub-Tec gold cast-on, Sub-Tec temporary abutment, Sub-Tec provisional PEEK abutment, Sub-Tec titanium abutment, Sub-Tec bar system (until Q2 2013), Sub-Tec CAD positioner, healing abutments, individual Ø 7	1
Prosthesis screw Sub-Tec <sup>Plus</sup>	57031			CAD SP, ST PMB, Sub-Tec <sup>Plus</sup> abutments (straight and angled), Sub-Tec CAD/CAM titanium adhesive abutment, Sub-Tec provisional titanium abutment, Sub-Tec bar system (from Q2 2013), Sub-Tec CAD/CAM TiBase L	1
Prosthesis screws Sub-Tec Universal	55534			Sub-Tec Universal	3.25–4.5
	55535			Sub-Tec Universal	5.5
Secondary screw Multi <sup>Plus</sup> (M1.4)	57534			Multi <sup>Plus</sup> System	1
Prosthesis screw Multi <sup>Plus</sup> (M1.8)	57535			Sub-Tec Multi <sup>Plus</sup> 20/30°	1







## OVERVIEW

CAD/CAM restoration	116
Impression taking and model fabrication	116
Crown restoration	117
Hybrid restoration	118
Screws	121

## CAD/CAM restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>CADP</b> comprising: <ul style="list-style-type: none"><li>• CAD positioner Mini</li><li>• prosthesis screw Mini</li></ul> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58256	■		Mini 2.7–3.1	1



## Impression taking and model fabrication

Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Open-tray impression for Mini</b> impression taking on implants on open trays comprising: <ul style="list-style-type: none"><li>• Mini impression post</li><li>• titanium screws L15 and L19</li></ul> Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2	56959	■		Mini 2.7–3.1	1



Implant analog					
Description	REF	Color code	Size	Compatibility	Units
<b>Model implant Mini</b>	56982	■		Mini 2.7–3.1	1



\*2 For torque specifications, see p. 128

\*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

## Crown restoration

<b>Solid abutment</b>					
Description	REF	Color code	Size	Compatibility	Units
<b>TiA</b> comprising: • titanium Mini abutment • prosthesis screw Mini • technician screw Mini Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57989	■		Mini 2.9–3.1	1
					
<b>Gold cast-on abutment</b>					
Description	REF	Color code	Size	Compatibility	Units
<b>Gold cast-on Mini</b> comprising: • cast-on abutment Mini • sub wax-up sleeve gold cast-on • prosthesis screw Mini, conical • technician screw Mini, conical Material: Gold/platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	57320	■		Mini 2.9–3.1	1
					
<b>Internal reamer gold cast-on Mini</b> For re-working the internal form fit (a technician screwdriver is recommended as the hold)	57323	■		Mini	1
					

## Hybrid restoration

Bar abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>TiBA</b> comprising: • titanium bar base Mini • prosthesis screw Mini • technician screw Mini Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm <small>*2</small>	57988	■		Mini 2.7–3.1	1



Easy-Con abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con Mini</b>	57623	■	L1.5	Mini 3.1	1
Material: Titanium alloy with TiN coating	57624	■	L2.5	Mini 3.1	1
Tool: Insert tool	57625	■	L3.5	Mini 3.1	1
<small>*3Locator®</small> <small>*2</small>					
<b>Insert tool Easy-Con/ 3Locator®</b> with ratchet connection	57008				1



Easy-Con impression taking					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con impression coping</b> (impression on Easy-Con)	57751				4
<b>Easy-Con analog</b>	57760				4



**Note:** Manufacturer notes about trade names, see page 125.

\*2 For torque specifications, see p. 128

## Hybrid restoration

Easy-Con female parts					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con laboratory set</b> comprising: <ul style="list-style-type: none"><li>• retention insert transparent, pink and blue</li><li>• block-out ring</li><li>• retention cap</li><li>• production insert, black</li></ul> Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
<b>Easy-Con instrument</b> For screw-fitting, removing, and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
<b>Easy-Con production insert (black)</b> Material: Polyamide (PA12)	57754				4
<b>Easy-Con retention insert (blue)</b> Withdrawal force approx.: 917g; 9N; 0–10°   Material: Polyamide (PA12)	57755				4
<b>Easy-Con retention insert (pink)</b> Withdrawal force approx.: 1427g; 14N; 0–10°   Material: Polyamide (PA12)	57756				4
<b>Easy-Con retention insert (transparent)</b> Withdrawal force approx.: 2243g; 22N; 0–10°   Material: Polyamide (PA12)	57757				4
<b>Easy-Con retention insert (red)</b> Withdrawal force approx.: 663g; 6.5N; 10-20°   Material: Polyamide (PA12)	57758				4
<b>Easy-Con retention insert (green)</b> Withdrawal force approx.: 2599g; 25.5N; 10-20° Material: Polyamide (PA12)	57759				4

Watch the video “BEGO Semados® Easy-Con System (chairside)”: <https://www.youtube.com/watch?v=JyfXzvLjwqU>



Watch the video “BEGO Semados® Easy-Con System (laboratory)”: <https://www.youtube.com/watch?v=JyfXzvLjwqU>



## Hybrid restoration

Ball attachment abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment Mini</b> Material: Titanium alloy Tool: Insert tool Ball attachment *2	56968	■	GH 1.5	Mini 2.9–3.1	1
	57055	■	GH 4	Mini 2.9–3.1	1
					
<b>Insert tool for ball attachment</b> with ratchet connection	55880				1
					
Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment impression set <sup>2</sup>Dalbo®-PLUS</b> impression on ball attachment comprising: <ul style="list-style-type: none"><li>• impression post cap for ball attachment (red)</li><li>• implant analog for ball attachment</li></ul>	55768				1
					
Ball attachment female parts <sup>2</sup> Dalbo®					
Description	REF	Color code	Size	Compatibility	Units
<b>Female parts <sup>2</sup>Dalbo®-PLUS</b> comprising: <ul style="list-style-type: none"><li>• female parts <sup>2</sup>Dalbo®-PLUS, complete (incl. retention insert)</li><li>• spacer</li></ul> Material: Titanium grade 4 Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator	55769				1
					
<b><sup>2</sup>Dalbo®-PLUS activator/deactivator</b>	55773				1
					
<b>Retention insert <sup>2</sup>Dalbo®-PLUS</b> Material: Precious metal Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator	55776				1
					

**Note:** Manufacturer notes about trade names, see page 125.

\*2 For torque specifications, see p. 128

## Screws

Prosthesis screws					
Description	REF	Color code	Size	Compatibility	Units
Prosthesis screw Mini	56983	■		TiA, TiBA, CADP (Mini)	1
Prosthesis screw Mini, conical	57321	■		Gold cast-on Mini	1







## OVERVIEW

Large-scale models

**124**

Demo material

**125**

## DEMO MODELS/MATERIAL

Large-scale models					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® SCX implant large-scale model	58242				1
					
BEGO Semados® RSX implant large-scale model	56750				1
					
BEGO Semados® RI* <sup>1</sup> implant large-scale model	58322				1
					
BEGO Semados® Mini implant large-scale model	57095				1
					
Acrylic block PS (large-scale model, scale 2:1) comprising:	56753				1
• acrylic block					
• one SCX and one RSX implant Ø 4.1 L11.5					
• PS TTiA (temporary abutment)					
• PS TiB (adhesive abutment)					
• PS TIAA, 15° P GH 1–2 (solid abutment)					
• PS TIAA, 20° E GH 2.5–4 (solid abutment)					
• prosthesis screw					
• hex screwdriver					
					

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

## DEMO MODELS/MATERIAL

### DEMO MODELS/MATERIAL

Demonstration material					
Description	REF	Color code	Size	Compatibility	Units
<b>Maxilla demonstration model</b> Clear acrylic model with implants	58243			SCX implants	1
	56755			RSX implants	1
<b>BEGO Semados® demo implants</b> incl. cover screw and titanium insertion post Material: Titanium (packaged non-sterile) Not for use on patients!	58244		SC		1
	58245		SCX		1
	56751		RS		1
	56752		RSX		1
	57699		RSX 3.0		1
	58345		RI* <sup>1</sup>		1
	55543		S		1
	55709		Mini		1
TJL (training jaw)	57464		Mandible		1
TJU (training jaw)	57465		Maxilla		1



**Note:**

<sup>2</sup>Dalbo® is a registered trademark of Cendres & Métaux SA, Biel/Bienne, Switzerland.

<sup>3</sup>Locator® is a registered trademark of ZEST Anchors LLC, CA, USA.

<sup>4</sup>DIM-Analog® is a registered trademark of nt-trading GmbH & Co. KG, Karlsruhe, Germany.





## OVERVIEW

Torque specifications	<b>128</b>
Material specifications	<b>130</b>
Index by article numbers	<b>138</b>
Alphabetical index	<b>152</b>

## USEFUL INFORMATION · TORQUE SPECIFICATIONS

Torques for BEGO Semados®	
Article name	Torque [Ncm]
Implant cover screw	10
Healing abutments	10
Healing abutments, individual	15
Impression post	10
CAD positioner (polyetheretherketone)	10
CAD positioner (grade 4 titanium)	15
CAD SP	15
<b>Temporary abutments</b>	<b>15</b>
• PS ITA Ø3.0–5.5 (temporary abutment) • PS PPA Ø3.25–5.5 (temporary abutment) • PS TPA Ø3.25–5.5 (temporary abutment) • PS TTiA/PS TTiA NH Ø3.25–5.5 (temporary abutment Hex/no Hex) • Sub-Tec temporary abutment (PEEK) • Sub-Tec provisional titanium abutment	
<b>Platform Switch System Ø3.0</b>	<b>20</b>
• PS TiA/PS TiAA Ø3.0 (solid abutment) • PS TiB Ø3.0 (adhesive abutment)	
<b>Platform Switch System Ø3.25–5.5</b>	<b>30</b>
• PS BA Ø3.25–4.5 (ball attachment abutment) • PS Easy-Con Ø3.75–4.5 (abutment) • PS PMB (milling blank, TI-Form milling blank) • PS TiB/PS TiB NH Ø3.25–5.5 (adhesive abutment Hex/no Hex) • PS OCP (restoration set) • PS GCO/PS GCO NH Ø3.25–5.5 (gold cast-on abutment Hex/no Hex) • PS Multi <sup>Plus</sup> Ø3.25–4.5 (post) • PS TiA/PS TiAA Ø3.75–5.5 (solid abutment) • PS UNI/PS UNI NH Ø3.25–5.5 (Universal abutment Hex/no Hex)	
<b>Platform Match System (Sub-System)</b>	<b>30</b>
• Sub-Tec ball attachment • Sub-Tec Easy-Con • ST PMB (milling blank) • Sub-Tec CAD/CAM TiBase L • Sub-Tec CAD/CAM titanium adhesive abutment • Sub-Tec gold cast-on • Sub-Tec Multi <sup>Plus</sup> abutment • Sub-Tec <sup>Plus</sup> titanium abutment • Sub-Tec Universal	
<b>Multi<sup>Plus</sup> System</b>	<b>20</b>
• Multi <sup>Plus</sup> titanium abutment • Multi <sup>Plus</sup> Universal	
<b>Mini System</b>	<b>25</b>
• Easy-Con Mini • Gold cast-on Mini • Ball attachment Mini • TiA (solid abutment) • TiBA (bar abutment)	

**Note:** Manufacturer notes about trade names, see page 125.

## General notes

To prevent damage to the components, original BEGO Implant Systems tools and products must be used for processing. The use of the torque ratchet in particular is required to comply with the prescribed initial tension of the connecting screws (specification stated in Ncm).

- Ensure that the prosthesis screws are not used in the laboratory and check that they have not been damaged.
- Once the implant abutments are finally screwed in, after about 5 to 10 minutes all connecting screws must be tightened/checked once more with the specified tightening torque.
- The implant/prosthesis interfaces must be regularly checked to ensure they are firmly seated and there are no gaps.
- If the components are exposed to extremely high loads, the screw(s) may loosen under some circumstances. The reasons for this must be identified and eliminated!
- It is recommended that implant abutments that are screwed in with a separate prosthesis screw are screwed in with a new prosthesis screw if the screw is loosened, for example, for cleaning the prosthetic restoration/implant abutments.

All specifications are determined to the best of our knowledge based on many years of practical applications and apply for restorations that have been executed in accordance with both our expertise and general scientific knowledge.

## General information about titanium

Titanium is a biopassive or bioinert substance that has an exceptionally neutral taste and is radiotransparent and resistant to corrosion as well as being a poor conductor of heat (thermal conductivity 0.168 to gold 3.118).

In implant dentistry, pure titanium and titanium alloys are processed while pure titanium also contains foreign components. Pure titanium is classified into 4 grades based on the proportion of foreign substances.

In all 4 groups, a maximum of 0.05% N, 0.08% C, and 0.015% H may be present. These substances are unavoidable because they are produced during the extraction of titanium or are deliberately introduced to control the physical properties.

Pure titanium (grades 1–4) and titanium alloys (from grade 5 onward) can be used for all dental work. It is possible to veneer crowns and bridges made of titanium with special ceramics, which, because of a phase transformation of the titanium at 882 °C (volume change), are fired at temperatures below 800 °C and must have a specific WAK (titanium: WAK of approx. 9.6).

When processing and polishing, the poor thermal conductivity of titanium must be heeded. During processing, heat may accumulate in localized areas, leading to increased O<sub>2</sub> deposits and in turn to embrittlement of the material.

Because titanium smears during machining, special mills must be used. Freshly polished surfaces only retain their mirror finish if they do not come into contact with H<sub>2</sub>O for at least 10 minutes.

During this time, they form a surface oxide that acts as a protective layer. When modelling frameworks, it must be noted that when casting titanium a thick, strong oxide layer develops with components of the investment material, which is known as the  $\alpha$  cast layer. This layer must be removed leaving no residue. Edges of models must be reinforced and are adjusted during the finishing. Titanium and titanium alloys can only be joined using welding (laser, plasma, arc, resistance).

Titanium				
Elements	Grade 2	Grade 3	Grade 4	Grade 5
Nitrogen, max. [%]	0.03	0.05	0.05	0.05
Carbon, max. [%]	0.08	0.08	0.08	0.08
Hydrogen, max. [%]	0.015	0.015	0.015	0.015
Iron, max. [%]	0.3	0.3	0.5	0.4
Oxygen, max. [%]	0.25	0.35	0.4	0.2
Aluminum [%]				5.5–6.75
Vanadium [%]				3.5–4.5
Titanium [%]	Remainder	Remainder	Remainder	Remainder

Compositions	
Material	Article
<b>Pure titanium grade 4</b> As per ASTM F67	BEGO Semados® S/SC/SCX/RS/RSX/RI/Mini implants CADP/CADP Multi <sup>Plus</sup> (CAD positioner) Implant cover screws Female parts <sup>2</sup> Dalbo®-PLUS, female parts PS CADP (CAD positioner) Sub-Tec CAD positioner TiBA (bar abutment)
<b>Titanium grade 5</b> (titanium alloy Ti-6Al-4V) As per ASTM F136	Impression post Healing abutment Selection set 0°/15°/20° BEGO Guide master sleeves/spoons BEGO Semados® Provisional Implant (PI) BEGO Semados® insertion posts on implants CAD SP (scansupport) Drill stops Easy-Con impression coping – cap, analog, retention cap Easy-Con Mini (titanium-nitride coating) Ball attachment Mini Model implants S/RS/RSX/RI/Mini Multi <sup>Plus</sup> healing posts, impressions, implant analogs, titanium abutment OCP A (implant analogs) Open-tray impression for Mini, Mini impression post PI bending tool, PI implant analog, PI multifunctional cap, PI paralleling post Prosthesis screws/technician screws PS BA (ball attachment abutment) PS BA (ball attachment abutment), spacer PS Easy-Con (abutment) (titanium-nitride coating) PS HP/PS HPW (healing abutment) PS ITA (temporary abutment) PS Multi <sup>Plus</sup> (post) PS OCP, OCP abutment (restoration set)

## USEFUL INFORMATION · MATERIAL SPECIFICATIONS

Compositions	
Material	Article
<b>Titanium grade 5</b> (titanium alloy Ti-6Al-4V) As per ASTM F136	DIM-Analog® body IDC (implant adjustment instrument) PS PMB (milling blank, TI-Form milling blank) PS TiA (solid abutments) PS TiAA (solid abutments) PS TiB/PS TiB NH (adhesive abutment) PS TTiA/PS TTiA NH (temporary abutment) PS UNI/PS UNI NH (Universal abutment Hex/no Hex), Universal base Hex/no Hex ST PMB (milling blank) Sub-Tec CAD/CAM TiBase L Sub-Tec CAD/CAM titanium adhesive abutment Hex/no Hex Sub-Tec Easy-Con abutment (titanium-nitride coating) Sub-Tec ball attachment Sub-Tec ball attachment, spacer Sub-Tec MultiPlus abutment Sub-Tec Universal/no Hex, Universal base Hex/no Hex Sub-TecPlus titanium abutment/titanium angulated abutment TiA (solid abutment)
<b>Stainless steel</b>	BEGO Guide preparation instruments/instruments, initial drills, tissue punches, bone shapers, pilot drills, pilot markers, depth drills, countersinks, threadformers, thread taps, shape drills, trepan drills DIM-Analog® knurled screw Paralleling post S/RS/RSX/RI/Mini Insert tool for implants Depth gauge Guiding wrench Drill extension PI removal tool/insert tool/stabilizer
<b>Polyetheretherketone (PEEK)</b>	Healing abutment, individual Ø 7 PI protection cap PS OCP (restoration set), multifunctional cap PS PPA/PS TPA (temporary abutment) Sub-Tec temporary abutment Ø 7, Sub-Tec provisional PEEK abutment
<b>60Au–19Pt–20Pd–1Ir</b>	Gold cast-on Mini, cast-on abutment Mini PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex), cast-on abutment Hex/no Hex Sub-Tec gold cast-on/no Hex, sub-cast-on abutment/no Hex
<b>69Au–12Ag–11Cu–4Pd–3Pt</b>	Female parts <sup>2</sup> Dalbo®-PLUS, retention insert <sup>2</sup> Dalbo-PLUS <sup>2</sup> Dalbo®-PLUS

**Note:** Manufacturer notes about trade names, see page 125.

Compositions	
Material	Article
<b>Polyoxymethylene (POM)</b>	Female parts <sup>2</sup> Dalbo®-PLUS, placeholder
	Multi <sup>Plus</sup> Universal, wax-up sleeve for gold cast-on
	PS CTI (impression set, closed tray), impression post cap
	PS UNI/PS UNI NH (Universal abutment Hex/no Hex), wax-up sleeve Universal
	Sub-Dent closed-tray impression, impression post cap
	Sub-Tec Universal/no Hex, sub-wax-up sleeve Universal
<b>Polycarbonate (PC)</b>	LCC, LCB (laboratory caps)
	PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex), wax-up sleeve for gold cast-on
	Sub-Tec gold cast-on/no Hex, sub-wax-up sleeve gold cast-on
<b>Polyamide (PA)</b>	Easy-Con impression coping, production insert
	Easy-Con retention insert

## NOTES

## NOTES



USEFUL INFORMATION · NOTES

## NOTES



## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
53735	Internal reamer for gold cast-on abutment	87, 105	55709	BEGO Semados® Mini demo implants	125
53872	Depth gauge, S/SC/SCX	64	55714	Initial drill, Mini implants	62
53888	Radiographic template, S implants	20	55715	Drill stops, S/SC/SCX 4.1	56
53897	Guiding wrench	63	55745	Radiographic template, RI implants	20
53948	Hexagon screwdriver 1.25mm, long, with ratchet connection	66	55746	Depth gauge, RI	64
53949	Hexagon screwdriver 1.25mm, short, with ratchet connection	66	55766	Threadformer, RI 3.25	61
53952	Slot screwdriver, long with ratchet connection	66	55768	Ball attachment impression set Dalbo®-PLUS	94, 112, 120
53999	Prosthesis screw Hex 1.25mm	95, 113	55769	Female parts Dalbo®-PLUS	94, 112, 120
55505	Implant cover screw, S 3.25	38	55773	Activator/deactivator Dalbo®-PLUS	94, 112, 120
55525	Sub-Tec Universal, S/RI 3.25–3.75	104	55776	Retention insert Dalbo®-PLUS	94, 112, 120
55526	Sub-Tec Universal no Hex, S/RI 3.25–3.75	104	55799	Ratchet/torque wrench	64, 66
55527	Sub-Tec Universal, S/RI 4.5	104	55804	Drill stops, depth drill 2.5 and S/SC/SCX 3.25–3.75	56
55528	Sub-Tec Universal no Hex, S/RI 4.5	104	55810	Drill stops, S/SC/SCX 4.5	56
55529	Sub-Tec Universal, S/RI 5.5	104	55815	Trepan drill, Ø 5.0 external/Ø 4.1 internal	64
55530	Sub-Tec Universal no Hex, S/RI 5.5	104	55816	Trepan drill, Ø 6.0 external/Ø 5.1 internal	64
55534	Prosthesis screw Sub-Tec Universal, S/RI 3.25–4.5	113	55817	Trepan drill, Ø 4.2 external/Ø 3.7 internal	64
55535	Prosthesis screw Sub-Tec Universal, S/RI 5.5	113	55826	Prosthetic kit	66
55536	Internal reamer Universal	86, 104	55830	Insert tool for implants, long, with ratchet connection	63
55537	External reamer Universal	86, 104	55831	Insert tool for implants, short, with ratchet connection	63
55539	Sub-Dent closed-tray impression, S/RI 3.75	100	55832	Insert tool for implants, long, with contra-angle connection	63
55540	Sub-Dent open-tray impression, S/RI 3.75	100	55860	Sub-Dent closed-tray impression, S 3.25	100
55543	BEGO Semados® S demo implants	125	55861	Sub-Dent open-tray impression, S 3.25	100
55551	Sub-Dent closed-tray impression, S/RI 5.5	100	55862	Sub-Tec gold cast-on, S/RI 3.25–3.75	105
55563	Hexagon screwdriver 1.25mm, short, contra-angle	66	55863	Paralleling post, S/SC/SCX	63
55564	Hexagon screwdriver 1.25mm, long, contra-angle	66	55873	Sub-Tec gold cast-on no Hex, S/RI 3.25–3.75	105
55590	Healing abutment, Ø 4.0 L3, S/RI 3.25–3.75	38	55880	Insert tool for ball attachment	94, 112, 120
55591	Healing abutment, Ø 4.0 L5, S/RI 3.25–3.75	38	55908	Implant cover screw, S/RI 5.5	38
55592	Healing abutment, Ø 4.0 L7, S/RI 3.25–3.75	38	55910	Drill stops, S/SC/SCX 5.5	56
55593	Healing abutment, Ø 5.0 L3, S/RI 3.25–4.5	38	55951	Sub-Tec temporary abutment Ø 7, S/RI 3.25–5.5	101
55594	Healing abutment, Ø 5.0 L5, S/RI 3.25–4.5	38	55953	Healing abutment, individual Ø 7, S/SC/SCX/RS/RSX/RI 3.25–5.5	33, 38
55595	Healing abutment, Ø 5.0 L7, S/RI 3.25–4.5	38	56300	Healing abutment, Ø 4.5 L3, S/RI 3.25–4.5	38
55599	BEGO Semados® ratchet adapter	43, 64, 66	56301	Healing abutment, Ø 4.5 L5, S/RI 3.25–4.5	38
55608	Implant cover screw, S/RI 3.75	38	56302	Healing abutment, Ø 4.5 L7, S/RI 3.25–4.5	38
55615	Implant cover screw, S/RI 4.1	38	56303	Healing abutment, Ø 6.0 L3, S/RI 3.25–5.5	38
55616	Implant cover screw, S/RI 4.5	38	56304	Healing abutment, Ø 6.0 L5, S/RI 3.25–5.5	38
55617	Sub-Dent closed-tray impression, S/RI 4.1	100	56305	Healing abutment, Ø 6.0 L7, S/RI 3.25–5.5	38
55618	Sub-Dent closed-tray impression, S/RI 4.5	100	56317	Sub-Tec gold cast-on, S/RI 4.5	105
55619	Sub-Dent open-tray impression, S/RI 4.1	100	56325	Sub-Tec gold cast-on no Hex, S/RI 4.5	105
55620	Sub-Dent open-tray impression, S/RI 4.5	100	56500	Sub-Dent open-tray impression, S/RI 5.5	100
55622	Sub-Tec Universal, S/RI 4.1	104	56515	Sub-Tec gold cast-on no Hex, S/RI 5.5	105
55623	Sub-Tec Universal no Hex, S/RI 4.1	104	56694	Model implant, 3.25	100
55624	Sub-Tec gold cast-on, S/RI 4.1	105			
55625	Sub-Tec gold cast-on no Hex, S/RI 4.1	105			

**Note:** Manufacturer notes about trade names, see page 125.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
56695	Model implant, S/RI 3.75	100	57103	Depth drill, long S/SC/SCX 3.25	55
56696	Model implant, S/RI 4.1	100	57104	Depth drill, short S/SC/SCX 3.75	55
56698	Model implant, S/RI 4.5	100	57105	Depth drill, long S/SC/SCX 3.75	55
56699	Model implant, S/RI 5.5	100	57106	Depth drill, short S/SC/SCX 4.1	55
56748	IDC, S/SC/SCX/RS/RSX/RI 3.25–5.5 (adjustment instrument)	63	57107	Depth drill, long S/SC/SCX 4.1	55
56749	IDC, RS/RSX 3.0 (adjustment instrument)	63	57108	Depth drill, short S/SC/SCX 4.5	55
56750	BEGO Semados® RSX implant large-scale model	124	57109	Depth drill, long S/SC/SCX 4.5	55
56751	BEGO Semados® RS demo implants	125	57110	Depth drill, short S/SC/SCX 5.5	55
56752	BEGO Semados® RSX demo implants	125	57116	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 3.25–3.75	102
56753	Acrylic block PS (large-scale model, scale 2:1)	124	57117	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 3.25–3.75	102
56755	Maxilla demonstration model, RSX implants	125	57120	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.1	102
56947	BEGO Semados® implant, Mini 2.7 L11.5	40	57121	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.1	102
56948	BEGO Semados® implant, Mini 2.7 L13	40	57124	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.5	102
56949	BEGO Semados® implant, Mini 2.7 L15	40	57125	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.5	102
56950	BEGO Semados® implant, Mini 2.9 L11.5	40	57128	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 5.5	102
56951	BEGO Semados® implant, Mini 2.9 L13	40	57129	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 5.5	102
56952	BEGO Semados® implant, Mini 2.9 L15	40	57130	BEGO Guide DS (drill sleeves)	52
56953	BEGO Semados® implant, Mini 3.1 L11.5	40	57132	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 1–2, S/RI 3.25–3.75	103
56954	BEGO Semados® implant, Mini 3.1 L13	40	57133	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 2.5–4, S/RI 3.25–3.75	103
56955	BEGO Semados® implant, Mini 3.1 L15	40	57134	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 3.25–3.75	103
56956	Implant cover screw Mini	40	57135	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 3.25–3.75	103
56957	Healing abutment Mini, Ø3.5 L3, Mini 2.7–3.1	40	57136	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.1	103
56958	Healing abutment Mini, Ø3.5 L4, Mini 2.7–3.1	40	57137	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.1	103
56959	Open-tray impression for Mini	116	57138	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.1	103
56968	Ball attachment Mini, GH 1.5, Mini 2.9–3.1	120	57139	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.1	103
56970	Mini-/Osseo <sup>Plus</sup> Tray, Mini 2.7–3.1	62	57140	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.5	103
56972	Paralleling post, Mini	63	57141	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.5	103
56979	Threadformer, Mini 2.7	62	57142	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.5	103
56980	Threadformer, Mini 2.9	62	57143	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.5	103
56981	Threadformer, Mini 3.1	62	57144	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 5.5	103
56982	Model implant Mini	116	57145	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 5.5	103
56983	Prosthesis screw Mini	121			
56990	Insert tool for implants, short, with contra-angle connection	63			
56991	Trepan drill, Ø5.0 external/Ø4.3 internal	64			
57008	Insert tool Easy-Con/Locator®	92, 110, 118			
57010	Radiographic template, Mini implants	20			
57031	Prosthesis screw Sub-Tec <sup>Plus</sup>	95, 113			
57055	Ball attachment Mini, GH 4, Mini 2.9–3.1	120			
57060	Sub-Tec CAD positioner, S/RI 3.25–5.5	98			
57095	BEGO Semados® Mini implant large-scale model	124			
57100	Depth drill 2.5, short S/SC/SCX	55			
57101	Depth drill 2.5, long S/SC/SCX	55			
57102	Depth drill, short S/SC/SCX 3.25	55			

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57146	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 5.5	103	57332	Thread tap, S/SC/SCX 3.25	55
57147	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 5.5	103	57333	Screw tap, S/SC/SCX 3.75	55
57221	BEGO Collagen Membrane, 15 × 20mm	12	57334	Screw tap, S/SC/SCX 4.1	55
57222	BEGO Collagen Membrane, 20 × 30mm	12	57335	Thread tap, S/SC/SCX 4.5	55
57223	BEGO Collagen Membrane, 30 × 40mm	12	57336	Screw tap, S/SC/SCX 5.5	55
57252	Healing abutment Mini, Ø3.5 L7, Mini 2.7–3.1	40	57340	BEGO Semados® tray <sup>Plus</sup> , S/SC/SCX 3.25–5.5	54
57265	Drill extension, one-part (without internal cooling)	63	57345	Drill stop Tray <sup>Plus</sup> , S/SC/SCX	56
57266	Hexagon screwdriver 1.25mm XS, with ratchet connection	66	57347	Drill module, S/SC/SCX 5.5	54
57285	Sub-Tec CAD/CAD titanium adhesive abutment, S/RI 3.25–3.75	98	57350	Countersink, S/SC/SCX 3.25	55
57286	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 3.25–3.75	98	57351	Countersink, S/SC/SCX 3.75	55
57287	Sub-Tec CAD/CAD titanium adhesive abutment, S/RI 4.1	98	57352	Countersink, S/SC/SCX 4.1	55
57288	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.1	98	57353	Countersink, S/SC/SCX 4.5	55
57289	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.5	98	57354	Countersink, S/SC/SCX 5.5	55
57290	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.5	98	57395	BEGO Guide master sleeves, Ø4.2 (A), S/SC/SCX/RS/RSX	46, 49
57291	Sub-Tec CAD/CAD titanium adhesive abutment, S/RI 5.5	98	57397	BEGO Guide master sleeves, Ø4.7 (B), S/SC/SCX/RS/RSX	46, 49
57292	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 5.5	98	57399	BEGO Guide Tray, S/SC/SCX 3.25–4.5	46
57300	Sub-Tec provisional titanium abutment no Hex, S/RI 3.25–3.75	101	57400	BEGO Guide – pilot drill, short	52
57301	Sub-Tec provisional titanium abutment no Hex, S/RI 4.1	101	57401	BEGO Guide – pilot drill, long	52
57302	Sub-Tec provisional titanium abutment no Hex, S/RI 4.5	101	57411	BEGO Guide spoon, Ø1.6 (A1), S/SC/SCX	46
57303	Sub-Tec provisional titanium abutment no Hex, S/RI 5.5	101	57412	BEGO Guide spoon, Ø2.5 (A2), S/SC/SCX	46
57304	Sub-Tec provisional titanium abutment, S/RI 3.25–3.75	101	57413	BEGO Guide spoon, Ø2.8 (A3), S/SC/SCX 3.25	46
57305	Sub-Tec provisional titanium abutment, S/RI 4.1	101	57414	BEGO Guide spoon, Ø3.25 (A4), S/SC/SCX 3.75	46
57306	Sub-Tec provisional titanium abutment, S/RI 4.5	101	57415	BEGO Guide spoon, Ø1.6 (B1), S/SC/SCX	46
57307	Sub-Tec provisional titanium abutment, S/RI 5.5	101	57416	BEGO Guide spoon, Ø2.5 (B2), S/SC/SCX	46
57308	Pilot marker, short, S/SC/SCX	54	57417	BEGO Guide spoon, Ø2.8 (B3), S/SC/SCX 3.25	46
57309	Pilot marker, long, S/SC/SCX	54	57418	BEGO Guide spoon, Ø3.25 (B4), S/SC/SCX 3.75	46
57320	Gold cast-on Mini, Mini 2.9–3.1	117	57419	BEGO Guide spoon, Ø3.65 (B5), S/SC/SCX 4.1	46
57321	Prosthesis screw Mini, conical	121	57420	BEGO Guide spoon, Ø4.0 (B6), S/SC/SCX 4.5	46
57323	Internal reamer for gold cast-on Mini	117	57421	BEGO Guide tissue punches, Ø4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	46, 49
57324	Healing abutment, conical, S/RI 3.25–3.75	38	57422	BEGO Guide tissue punches, Ø4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	46, 49
			57423	BEGO Guide pilot drill, Ø1.6 L18 (X1), S/SC/SCX	47
			57424	BEGO Guide pilot drill, Ø1.6 L23.5 (Y1), S/SC/SCX	47
			57425	BEGO Guide pilot drill, Ø1.6 L29 (Z1), S/SC/SCX	47

**Note:** Manufacturer notes about trade names, see page 125.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57426	BEGO Guide depth drill Ø 2.5, L18 (X2), S/SC/SCX	47	57451	BEGO Guide spoon, Ø 4.2 (AY), S/SC/SCX	48
57427	BEGO Guide depth drill, Ø 2.5 L23.5 (Y2), S/SC/SCX	47	57452	BEGO Guide spoon, Ø 4.2 (AZ), S/SC/SCX	48
57428	BEGO Guide depth drill Ø 2.5, L29 (Z2), S/SC/SCX	47	57453	BEGO Guide spoon, Ø 4.7 (BX), S/SC/SCX	48
57429	BEGO Guide depth drill Ø 2.8, L18 (X3), S/SC/SCX 3.25	47	57454	BEGO Guide spoon, Ø 4.7 (BY), S/SC/SCX	48
57430	BEGO Guide depth drill Ø 2.8 L23.5 (Y3), S/SC/SCX 3.25	47	57455	BEGO Guide spoon, Ø 4.7 (BZ), S/SC/SCX	48
57431	BEGO Guide depth drill Ø 2.8, L29 (Z3), S/SC/SCX 3.25	47	57456	BEGO Guide depth stop ring connector, Ø 4.2 (A), S/SC/SCX/RS/RSX	48, 51
57432	BEGO Guide depth drill Ø 3.25, L18 (X4), S/SC/SCX 3.75	47	57457	BEGO Guide depth stop ring connector, Ø 4.7 (B), S/SC/SCX/RS/RSX	48, 51
57433	BEGO Guide Pilot Ø 3.25 L23.5 (Y4), S/SC/SCX 3.75	47	57458	BEGO Guide ratchet adapter for connector, S/SC/SCX	48
57434	BEGO Guide depth drill Ø 3.25, L29 (Z4), S/SC/SCX 3.75	47	57459	BEGO Guide center drill, Ø 4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	47, 50
57435	BEGO Guide depth drill Ø 3.65, L18 (X5), S/SC/SCX 4.1	47	57463	BEGO Guide center drill, Ø 4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	47, 50
57436	BEGO Guide Pilot Ø 3.65 L23.5 (Y5), S/SC/SCX 4.1	47	57465	TJU (training jaw) for maxilla	125
57437	BEGO Guide depth drill Ø 3.65, L29 (Z5), S/SC/SCX 4.1	47	57464	TJL (training jaw) for mandible	125
57438	BEGO Guide depth drill Ø 4.0, L18 (X6), S/SC/SCX 4.5	47	57476	Drill stops for depth drill 2.5 RS/RSX	59
57439	BEGO Guide Pilot Ø 4.0 L23.5 (Y6), S/SC/SCX 4.5	47	57477	Drill stops, RS/RSX 3.0	59
57441	BEGO Guide depth drill Ø 4.0, L29 (Z6), S/SC/SCX 4.5	47	57478	Drill stops, RS/RSX 3.75	59
57442	BEGO Guide countersink, (3), S/SC/SCX 3.25	47	57479	Drill stops, RS/RSX 4.1–4.5	59
57443	BEGO Guide Countersink, (4), S/SC/SCX 3.75	47	57480	Drill stops, RS/RSX 5.5	59
57444	BEGO Guide Countersink, (5), S/SC/SCX 4.1	47	57481	Pilot marker, short, RS/RSX	57
57445	BEGO Guide Countersink, (6), S/SC/SCX 4.5	47	57482	Pilot marker, long, RS/RSX	57
57446	BEGO Guide thread tap, (3), S/SC/SCX 3.25	48	57483	Drill stop Tray <sup>Plus</sup> , RS/RSX	59
57447	BEGO Guide screw tap, (4), S/SC/SCX 3.75	48	57484	DD D1, RS/RSX 3.0 (depth drill)	58
57448	BEGO Guide screw tap, (5), S/SC/SCX 4.1	48	57485	DD D1, RS/RSX 3.75 (depth drill)	58
57449	BEGO Guide thread tap, (6), S/SC/SCX 4.5	48	57486	DD D1, RS/RSX 4.1 (depth drill)	58
57450	BEGO Guide spoon, Ø 4.2 (AX), S/SC/SCX	48	57487	DD D1, RS/RSX 4.5 (depth drill)	58
			57488	DD D1, RS/RSX 5.5 (depth drill)	58
			57494	Sub-Tec provisional PEEK abutment, S/RI 3.25–3.75	101
			57495	Sub-Tec provisional PEEK abutment, S/RI 4.1–4.5	101
			57500	BEGO Semados® implant, S 3.25 L8.5	36
			57501	BEGO Semados® implant, S 3.25 L10	36
			57502	BEGO Semados® implant, S 3.25 L11.5	36
			57503	BEGO Semados® implant, S 3.25 L13	36
			57505	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 3.25–3.75	106
			57506	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.1	106
			57507	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.5	106
			57508	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 3.25–3.75	106
			57509	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.1	106
			57510	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.5	106

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57511	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 3.25–3.75	107	57593	Countersink, RI 4.1	61
57512	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.1	107	57594	Countersink, RI 4.5	61
57513	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.5	107	57595	Countersink, RI 5.5	61
57514	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 3.25–3.75	107	57598	Paralleling post, RI	63
57515	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.1	107	57601	BEGO Semados® implant, S 3.75 L8.5	36
57516	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.5	107	57602	BEGO Semados® implant, S 3.75 L10	36
57517	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 3.25–3.75	107	57603	BEGO Semados® implant, S 3.75 L11.5	36
57518	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.1	107	57604	BEGO Semados® implant, S 3.75 L13	36
57519	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.5	107	57612	BEGO Semados® Tray <sup>Plus</sup> , RI 3.75–5.5	60
57520	Multi <sup>Plus</sup> healing post	89, 107	57613	Drill module, RI 5.5	60
57521	Multi <sup>Plus</sup> healing post, Mushroom	89, 107	57615	Threadformer, RI 3.75	61
57522	Multi <sup>Plus</sup> closed-tray impression, short	90, 108	57616	Threadformer, RI 4.1	61
57523	Multi <sup>Plus</sup> open-tray impression	90, 108	57617	Threadformer, RI 4.5	61
57524	Multi <sup>Plus</sup> implant analog, 1 unit	90, 108	57618	Threadformer, RI 5.5	61
57525	Multi <sup>Plus</sup> implant analog, 4 units	90, 108	57619	Thread tap, RI 3.75	61
57526	Multi <sup>Plus</sup> titanium abutment	91, 109	57620	Screw tap, RI 4.1	61
57530	Multi <sup>Plus</sup> alignment aid, 20°	88, 106	57621	Screw tap, RI 4.5	61
57531	Multi <sup>Plus</sup> alignment aid, 30°	88, 106	57622	Thread tap, RI 5.5	61
57532	Multi <sup>Plus</sup> insertion splint	88, 106	57623	Easy-Con Mini, L1.5, Mini 3.1	118
57533	Insertion instrument Multi <sup>Plus</sup> abutment 0°	88, 106	57624	Easy-Con Mini, L2.5, Mini 3.1	118
57534	Secondary screw Multi <sup>Plus</sup> (M1.4)	95, 113	57625	Easy-Con Mini, L3.5, Mini 3.1	118
57535	Secondary screw Multi <sup>Plus</sup> (M1.8)	95, 113	57631	Sub-Tec ball attachment, GH 0, S/RI 3.25–3.75	112
57538	Multi <sup>Plus</sup> Universal	91, 109	57632	Sub-Tec ball attachment, GH 0, S/RI 4.1–4.5	112
57539	External reamer Multi <sup>Plus</sup>	91, 109	57633	Sub-Tec ball attachment, GH 3, S/RI 3.25–3.75	112
57540	Internal reamer Multi <sup>Plus</sup>	91, 109	57634	Sub-Tec ball attachment, GH 3, S/RI 4.1–4.5	112
57554	Multi <sup>Plus</sup> closed-tray impression, long	90, 108	57635	Sub-Tec ball attachment, GH 5, S/RI 3.25–3.75	112
57581	Pilot marker, short, RI	60	57636	Sub-Tec ball attachment, GH 5, S/RI 4.1–4.5	112
57582	Pilot marker, long, RI	60	57656	Sub-Tec CAD/CAM TiBase L, S/RI 3.25–3.75	99
57583	Depth drill 3.2, short RI	60	57657	Sub-Tec CAD/CAM TiBase L, S/RI 4.1	99
57584	Depth drill 3.2, long RI	60	57658	Sub-Tec CAD/CAM TiBase L, S/RI 4.5	99
57585	Depth drill, short RI 3.75	61	57659	Sub-Tec CAD/CAM TiBase L, S/RI 5.5	99
57586	Depth drill, long RI 3.75	61	57660	BEGO Semados® Provisional Implant (PI), 1 unit	42
57587	Depth drill, short RI 4.1	61	57661	PI multifunctional cap, 1 unit	42
57588	Depth drill, long RI 4.1	61	57662	PI protection cap	42
57589	Depth drill, short RI 4.5	61	57663	PI paralleling post	43
57590	Depth drill, long RI 4.5	61	57664	PI depth drill	43
57591	Depth drill, short RI 5.5	61	57665	PI insert tool	43
57592	Countersink, RI 3.75	61	57666	PI removal tool	43
			57667	PI bending instrument	43
			57668	PI ratchet	43
			57669	PI stabilizer	43
			57670	BEGO Semados® PI tray	42
			57671	PI implant analog	42
			57672	Radiographic template, PI implants	20
			57673	BEGO Semados® Provisional Implant (PI), 10 units	42

**Note:** Manufacturer notes about trade names, see page 125.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57674	PI multifunctional cap, 5 units	42	57718	BEGO Semados® implant, RI 4.1 L8.5	30
57686	BEGO Guide Sp, Ø2.0 (A1), RS/RSX (reduction sleeve)	49	57719	BEGO Semados® implant, RI 4.1 L10	30
57687	BEGO Guide Sp, Ø2.5 (A2), RS/RSX (reduction sleeve)	49	57720	BEGO Semados® implant, RI 4.1 L11.5	30
57688	BEGO Guide Sp, Ø2.8 (A3), RS/RSX 3.0 (reduction sleeve)	49	57721	BEGO Semados® implant, RI 4.1 L13	30
57689	BEGO Guide Sp, Ø3.4 (A4), RS/RSX 3.75 (reduction sleeve)	49	57723	BEGO Guide DD, Ø2.8 L29 (Z3), RS/RSX 3.0 (depth drill)	50
57690	BEGO Guide Sp, Ø2.0 (B1), RS/RSX (reduction sleeve)	49	57724	BEGO Guide DD, Ø3.4 L18 (X4), RS/RSX 3.75 (depth drill)	50
57691	BEGO Guide Sp, Ø2.5 (B2), RS/RSX (reduction sleeve)	49	57725	BEGO Guide DD, Ø3.4 L23.5 (Y4), RS/RSX 3.75 (depth drill)	50
57692	BEGO Guide Sp, Ø2.8 (B3), RS/RSX 3.0 (reduction sleeve)	49	57726	BEGO Guide DD, Ø3.4 L29 (Z4), RS/RSX 3.75 (depth drill)	50
57693	BEGO Guide Sp, Ø3.4 (B4), RS/RSX 3.75 (reduction sleeve)	49	57727	BEGO Guide DD, Ø3.8 L18 (X5), RS/RSX 4.1 (depth drill)	50
57694	BEGO Guide Sp, Ø3.8 (B5), RS/RSX 4.1 (reduction sleeve)	49	57728	BEGO Semados® implant, RI 4.5 L8.5	30
57695	BEGO Guide Sp, Ø4.1 (B6), RS/RSX 4.5 (reduction sleeve)	49	57729	BEGO Semados® implant, RI 4.5 L10	30
57696	BEGO Guide PD, Ø2.0 L18 (X1), RS/RSX (pilot drill)	50	57730	BEGO Semados® implant, RI 4.5 L11.5	30
57697	BEGO Guide pilot drill, Ø2.0 L23.5 (Y1), RS/RSX (pilot drill)	50	57731	BEGO Semados® implant, RI 4.5 L13	30
57698	BEGO Guide PD, Ø2.0 L29 (Z1), RS/RSX (pilot drill)	50	57733	BEGO Guide DD, Ø3.8 L23.5 (Y5), RS/RSX 4.1 (depth drill)	50
57699	BEGO Semados® RSX demo implants 3.0	125	57734	BEGO Guide DD, Ø3.8 L29 (Z5), RS/RSX 4.1 (depth drill)	50
57700	BEGO Semados® implant, S 4.5 L7	36	57735	BEGO Guide DD, Ø4.1 L18 (X6), RS/RSX 4.5 (depth drill)	50
57701	BEGO Semados® implant, S 4.5 L8.5	36	57736	BEGO Guide DD, Ø4.1 L23.5 (Y6), RS/RSX 4.5 (depth drill)	50
57702	BEGO Semados® implant, S 4.5 L10	36	57737	BEGO Guide DD, Ø4.1 L29 (Z6), RS/RSX 4.5 (depth drill)	50
57703	BEGO Semados® implant, S 4.5 L11.5	36	57738	BEGO Semados® implant, RI 5.5 L8.5	30
57704	BEGO Semados® implant, S 4.5 L13	36	57739	BEGO Semados® implant, RI 5.5 L10	30
57708	BEGO Semados® implant, RI 3.75 L8.5	30	57740	BEGO Semados® implant, RI 5.5 L11.5	30
57709	BEGO Semados® implant, RI 3.75 L10	30	57741	BEGO Semados® implant, RI 5.5 L13	30
57710	BEGO Semados® implant, RI 3.75 L11.5	30	57743	Sub-Tec Easy-Con abutment, L1, S/RI 3.75–4.1	110
57711	BEGO Semados® implant, RI 3.75 L13	30	57744	Sub-Tec Easy-Con abutment, L2, S/RI 3.75–4.1	110
57713	BEGO Guide PD, Ø2.5 L18 (X2), RS/RSX (depth drill)	50	57745	Sub-Tec Easy-Con abutment, L3, S/RI 3.75–4.1	110
57714	BEGO Guide pilot drill, Ø2.5 L23.5 (Y2), RS/RSX (depth drill)	50	57746	Sub-Tec Easy-Con abutment, L4, S/RI 3.75–4.1	110
57715	BEGO Guide PD, Ø2.5 L29 (Z2), RS/RSX (depth drill)	50	57747	Sub-Tec Easy-Con abutment, L1, S/RI 4.5	110
57716	BEGO Guide DD, Ø2.8 L18 (X3), RS/RSX 3.0 (depth drill)	50	57748	Sub-Tec Easy-Con abutment, L2, S/RI 4.5	110
57717	BEGO Guide DD, Ø2.8 L23.5 (Y3), RS/RSX 3.0 (depth drill)	50	57749	Sub-Tec Easy-Con abutment, L3, S/RI 4.5	110
			57750	Sub-Tec Easy-Con abutment, L4, S/RI 4.5	110
			57751	Easy-Con impression coping	92, 110, 118
			57752	Easy-Con laboratory set	93, 111, 119
			57753	Easy-Con instrument	93, 111, 119
			57754	Easy-Con production insert (black)	93, 111, 119
			57755	Easy-Con retention insert (blue)	93, 111, 119
			57756	Easy-Con retention insert (pink)	93, 111, 119
			57757	Easy-Con retention insert (transparent)	93, 111, 119

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57758	Easy-Con retention insert (red)	93, 111, 119	57811	PS HP, Ø 5.5 L3, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	32
57759	Easy-Con retention insert (green)	93, 111, 119	57812	PS HP, Ø 5.5 L5, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	32
57760	Easy-Con analog	92, 110, 118	57813	PS HP, Ø 6.5 L3, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	32
57764	PS HP, Ø 3.0 L3, RS/RSX 3.0 (healing abutment)	32	57814	PS HP, Ø 6.5 L5, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	32
57765	PS HP, Ø 3.0 L5, RS/RSX 3.0 (healing abutment)	32	57815	PS HPW, Ø 5.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	33
57766	PS HP, Ø 3.0 L7, RS/RSX 3.0 (healing abutment)	32	57816	PS HPW, Ø 6.0 L3, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	33
57767	PS HP, Ø 4.0 L3, RS/RSX 3.0 (healing abutment)	32	57817	PS HPW, Ø 6.5 L3, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	33
57768	PS HP, Ø 4.0 L5, RS/RSX 3.0 (healing abutment)	32	57818	PS HPW, Ø 7.0 L3, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	33
57769	PS HP, Ø 4.0 L7, RS/RSX 3.0 (healing abutment)	32	57819	PS IMPA, SC/SCX/RS/RSX/RI*1 3.75 (implant analog)	80
57773	PS CTI, RS/RSX 3.0 (impression set, closed)	80	57820	PS IMPA, SC/SCX/RS/RSX/RI*1 4.1 (implant analog)	80
57774	PS CTI, RS/RSX 3.0 (impression set, open)	80	57821	PS IMPA, SC/SCX/RS/RSX/RI*1 4.5 (implant analog)	80
57776	PS TiA, GH 2.5–4, RS/RSX 3.0 (solid abutment)	81	57822	PS IMPA, SC/SCX/RS/RSX/RI*1 5.5 (implant analog)	80
57778	PS ITA, RS/RSX 3.0 (temporary abutment)	81	57823	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment)	77
57781	PS TiB, RS/RSX 3.0 (adhesive abutment)	76	57824	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment)	77
57782	Pscrew (prosthesis screw Ø 3.0)	95	57825	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment)	77
57784	Pscrew (prosthesis screw, for CAD positioner Ø 3.0)	95	57826	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment)	77
57796	PS IMPA, RS/RSX 3.0 (implant analog)	80	57827	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment no Hex)	78
57797	PS TiAA, 15° P GH 2.5–4, RS/RSX 3.0 (solid abutment)	81	57828	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment no Hex)	78
57798	PS TiAA, 15° E GH 2.5–4, RS/RSX 3.0 (solid abutment)	81	57829	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment no Hex)	78
57799	PS CTI, SC/SCX/RS/RSX/RI*1 3.75 (impression set, closed)	80	57830	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment no Hex)	78
57800	PS CTI, SC/SCX/RS/RSX/RI*1 4.1 (impression set, closed)	80	57831	PS UNI, SC/SCX/RS/RSX/RI*1 3.25–3.75 (Universal abutment)	86
57801	PS CTI, SC/SCX/RS/RSX/RI*1 4.5 (impression set, closed)	80	57832	PS UNI, SC/SCX/RS/RSX/RI*1 4.1 (Universal abutment)	86
57802	PS CTI, SC/SCX/RS/RSX/RI*1 5.5 (impression set, closed)	80	57833	PS UNI, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment)	86
57803	PS OTI, SC/SCX/RS/RSX/RI*1 3.75 (impression set, open)	80			
57804	PS OTI, SC/SCX/RS/RSX/RI*1 4.1 (impression set, open)	80			
57805	PS OTI, SC/SCX/RS/RSX/RI*1 4.5 (impression set, open)	80			
57806	PS OTI, SC/SCX/RS/RSX/RI*1 5.5 (impression set, open)	80			
57807	PS HP, Ø 4.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	32			
57808	PS HP, Ø 4.5 L5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	32			
57809	PS HP, Ø 5.0 L3, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	32			
57810	PS HP, Ø 5.0 L5, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	32			

**Note:** Manufacturer notes about trade names, see page 125.

\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57834	PS UNI, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (Universal abutment)	86	57862	BEGO Semados® implant, RSX 3.0 L10	27
57835	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (Universal no Hex abutment)	86	57863	BEGO Semados® implant, RSX 3.0 L11.5	27
57836	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (Universal abutment no Hex)	86	57864	BEGO Semados® implant, RSX 3.0 L13	27
57837	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (Universal abutment no Hex)	86	57866	BEGO Semados® implant, RSX 3.75 L8.5	27
57838	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (Universal abutment no Hex)	86	57867	BEGO Semados® implant, RSX 3.75 L10	27
57840	BEGO Semados® implant, S 4.1 L7	36	57868	BEGO Semados® implant, RSX 3.75 L11.5	27
57841	BEGO Semados® implant, S 4.1 L8.5	36	57869	BEGO Semados® implant, RSX 3.75 L13	27
57842	BEGO Semados® implant, S 4.1 L10	36	57870	BEGO Semados® implant, RSX 3.75 L15	27
57843	BEGO Semados® implant, S 4.1 L11.5	36	57871	BEGO Semados® implant, RSX 4.1 L7	27
57844	BEGO Semados® implant, S 4.1 L13	36	57872	BEGO Semados® implant, RSX 4.1 L8.5	27
57846	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	83	57873	BEGO Semados® implant, RSX 4.1 L10	27
57847	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	83	57874	BEGO Semados® implant, RSX 4.1 L11.5	27
57848	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	83	57875	BEGO Semados® implant, RSX 4.1 L13	27
57849	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	83	57876	BEGO Semados® implant, RSX 4.1 L15	27
57850	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	83	57877	BEGO Semados® implant, RSX 4.5 L7	27
57851	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	83	57878	BEGO Semados® implant, RSX 4.5 L8.5	27
57852	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	83	57879	BEGO Semados® implant, RSX 4.5 L10	27
57853	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	83	57880	BEGO Semados® implant, RSX 4.5 L11.5	27
57854	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	82	57881	BEGO Semados® implant, RSX 4.5 L13	27
57855	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	82	57882	BEGO Semados® implant, RSX 4.5 L15	27
57856	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (provisional abutment)	82	57883	BEGO Semados® implant, RSX 5.5 L7	27
57857	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment)	82	57884	BEGO Semados® implant, RSX 5.5 L8.5	27
57858	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment no Hex)	82	57885	BEGO Semados® implant, RSX 5.5 L10	27
57859	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment no Hex)	82	57886	BEGO Semados® implant, RSX 5.5 L11.5	27
57860	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (provisional abutment no Hex)	82	57887	BEGO Semados® implant, RSX 5.5 L13	27
57861	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment no Hex)	82	57889	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
			57890	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
			57891	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
			57892	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
			57893	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
			57894	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
			57895	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
			57896	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
			57897	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84
			57898	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57899	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84	57922	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	85
57900	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84	57923	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	85
57901	BEGO Semados® implant, S 5.5 L8.5	36	57924	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	85
57902	BEGO Semados® implant, S 5.5 L10	36	57926	Depth drill 2.5 short, RS/RSX	57
57903	BEGO Semados® implant, S 5.5 L11.5	36	57927	Depth drill 2.5 long, RS/RSX	57
57904	BEGO Semados® implant, S 5.5 L13	36	57928	Depth drill short, RS/RSX 3.0	58
57905	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84	57929	Depth drill long, RS/RSX 3.0	58
57906	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84	57930	Depth drill short, RS/RSX 3.75	58
57907	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84	57931	Depth drill long, RS/RSX 3.75	58
57908	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84	57932	Depth drill short, RS/RSX 4.1	58
57909	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	85	57933	Depth drill long, RS/RSX 4.1	58
57910	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	85	57934	Depth drill short, RS/RSX 4.5	58
57911	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	85	57935	Depth drill long, RS/RSX 4.5	58
57912	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	85	57936	Depth drill short, RS/RSX 5.5	58
57913	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	85	57937	Countersink, RS/RSX 3.0	58
57914	PS TiAA, 20° P GH 2.5–4, SC/SCX/S/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	85	57938	Countersink, RS/RSX 3.75	58
57915	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	85	57939	Countersink, RS/RSX 4.1	58
57916	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	85	57940	Countersink, RS/RSX 4.5	58
57917	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	85	57941	Countersink, RS/RSX 5.5	58
57918	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	85	57943	Thread tap, RS/RSX 3.0	58
57919	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	85	57944	Thread tap, RS/RSX 3.75	58
57920	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	85	57945	Screw tap, RS/RSX 4.1	58
57921	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	85	57946	Thread tap, RS/RSX 4.5	58
			57947	Thread tap, RS/RSX 5.5	58
			57948	Drill module, RS/RSX 5.5	57
			57949	BEGO Semados® Tray <sup>Plus</sup> , RS/RSX 3.0–5.5	57
			57950	Implant cover screw, RS/RSX 3.0	32
			57951	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	32
			57952	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	32
			57953	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	32
			57954	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	32
			57955	Depth gauge, RS/RSX	64
			57956	Paralleling post, RS/RSX	63
			57959	Radiographic template, RS/RSX implants	20
			57962	BEGO Semados® implant, RS 3.0 L10	26
			57963	BEGO Semados® implant, RS 3.0 L11.5	26
			57964	BEGO Semados® implant, RS 3.0 L13	26
			57966	BEGO Semados® implant, RS 3.75 L8.5	26

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57967	BEGO Semados® implant, RS 3.75 L10	26	58061	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AZ), RS/RSX (connector)	51
57968	BEGO Semados® implant, RS 3.75 L11.5	26	58062	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BX), RS/RSX (connector)	51
57969	BEGO Semados® implant, RS 3.75 L13	26	58063	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BY), RS/RSX (connector)	51
57970	BEGO Semados® implant, RS 3.75 L15	26	58064	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BZ), RS/RSX (connector)	51
57971	BEGO Semados® implant, RS 4.1 L7	26	58065	BEGO Guide Conn, with ratchet connection, Ø4.2 (AX), RS/RSX (connector)	51
57972	BEGO Semados® implant, RS 4.1 L8.5	26	58066	BEGO Guide Conn, with ratchet connection, Ø4.2 (AY), RS/RSX (connector)	51
57973	BEGO Semados® implant, RS 4.1 L10	26	58067	BEGO Guide Conn, with ratchet connection, Ø4.2 (AZ), RS/RSX (connector)	51
57974	BEGO Semados® implant, RS 4.1 L11.5	26	58068	BEGO Guide Conn, with ratchet connection, Ø4.7 (BX), RS/RSX (connector)	51
57975	BEGO Semados® implant, RS 4.1 L13	26	58069	BEGO Guide Conn, with ratchet connection, Ø4.7 (BY), RS/RSX (connector)	51
57976	BEGO Semados® implant, RS 4.1 L15	26	58070	BEGO Guide Conn, with ratchet connection, Ø4.7 (BZ), RS/RSX (connector)	51
57977	BEGO Semados® implant, RS 4.5 L7	26	58071	BEGO Guide Tr, RS/RSX 3.0–4.5 (surgical tray)	49
57978	BEGO Semados® implant, RS 4.5 L8.5	26	58072	PS PPA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	82
57979	BEGO Semados® implant, RS 4.5 L10	26	58073	PS PPA SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	82
57980	BEGO Semados® implant, RS 4.5 L11.5	26	58074	PS PPA SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment)	82
57981	BEGO Semados® implant, RS 4.5 L13	26	58075	PS PPA SC/SCX/RS/RSX/RI*1 5.5 (temporary abutment)	82
57982	BEGO Semados® implant, RS 4.5 L15	26	58076	PS ITA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	82
57983	BEGO Semados® implant, RS 5.5 L7	26	58077	PS ITA SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	82
57984	BEGO Semados® implant, RS 5.5 L8.5	26	58078	PS ITA SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment)	82
57985	BEGO Semados® implant, RS 5.5 L10	26	58088	PS TiA, conical, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	83
57986	BEGO Semados® implant, RS 5.5 L11.5	26	58089	PS TiA, conical, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	83
57987	BEGO Semados® implant, RS 5.5 L13	26	58090	PS TiA, conical, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	83
57988	TiBA, Mini 2.7–3.1 (bar abutment)	118	58091	PS TiA, conical, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	83
57989	TiA, Mini 2.9–3.1 (solid abutment)	117	58092	PS GCO, SC/SCX/RS/RSX/RI*1 3.25–3.75 (gold cast-on abutment)	87
57993	PS UNI PScrew (prosthesis screw)	95	58093	PS GCO SC/SCX/RS/RSX/RI*1 4.1 (gold cast-on abutment)	87
57995	DD, Mini 2.7 (depth drill)	62			
57996	DD, Mini 2.9 (depth drill)	62			
57997	DD, Mini 3.1 (depth drill)	62			
58051	BEGO Guide CS, (3), RS/RSX 3.0 (countersink)	50			
58052	BEGO Guide System (4) RS/RSX 3.75 (countersink)	50			
58053	BEGO Guide System (5) RS/RSX 4.1 (countersink)	50			
58054	BEGO Guide System (6) RS/RSX 4.5 (countersink)	50			
58055	BEGO Guide ST, (3), RS/RSX 3.0 (thread tap)	51			
58056	BEGO Guide ST, (4), RS/RSX 3.75 (thread tap)	51			
58057	BEGO Guide ST, (5), RS/RSX 4.1 (thread tap)	51			
58058	BEGO Guide ST (6) RS/RSX 4.5 (thread tap)	51			
58059	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AX), RS/RSX (connector)	51			
58060	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AY), RS/RSX (connector)	51			

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58094	PS GCO SC/SCX/RS/RSX/RI*1 4.5 (gold cast-on abutment)	87	58123	PS BA, GH0, SC/SCX/RS/RSX/RI*1 4.1 (ball attachment abutment)	94
58096	PS GCO NH, SC/SCX/RS/RSX/RI*1 3.25–3.75 (gold cast-on abutment no Hex)	87	58124	PS BA GH3, SC/SCX/RS/RSX/RI*1 4.1 (ball attachment abutment)	94
58097	PS GCO NH, SC/SCX/RS/RSX/RI*1 4.1 (gold cast-on abutment no Hex)	87	58125	PS BA, GH5, SC/SCX/RS/RSX/RI*1 4.1 (ball attachment abutment)	94
58098	PS GCO NH, SC/SCX/RS/RSX/RI*1 4.5 (gold cast-on abutment no Hex)	87	58126	PS BA, GH0, SC/SCX/RS/RSX/RI*1 4.5 (ball attachment abutment)	94
58099	PS GCO NH, SC/SCX/RS/RSX/RI*1 5.5 (gold cast-on abutment no Hex)	87	58127	PS BA, GH3, SC/SCX/RS/RSX/RI*1 4.5 (ball attachment abutment)	94
58100	PS MultiPlus, 0° GH 1, SC/SCX/RS/RSX/RI*1 3.25–3.75 (abutment)	88	58128	PS BA, GH5, SC/SCX/RS/RSX/RI*1 4.5 (ball attachment abutment)	94
58101	PS MultiPlus, 0° GH 3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (abutment)	88	58130	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	92
58102	PS MultiPlus, 0° GH 1, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	88	58131	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	92
58103	PS MultiPlus, 0° GH 3, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	88	58132	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	92
58104	PS MultiPlus, 0° GH 1, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	88	58133	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	92
58105	PS MultiPlus, 0° GH 3, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	88	58134	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	92
58108	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI*1 3.25–3.75 (abutment)	89	58135	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	92
58109	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (abutment)	89	58136	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	92
58110	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	89	58137	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	92
58111	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	89	58138	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	92
58112	PS MultiPlus, 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	89	58139	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	92
58113	PS MultiPlus, 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	89	58140	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	92
58116	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (abutment)	89	58141	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	92
58117	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	89	58142	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 5.5 (abutment)	92
58118	PS MultiPlus, 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	89	58143	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 5.5 (abutment)	92
58120	PS BA, GH0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (ball attachment abutment)	94	58146	PS TPA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	82
58121	PS BA GH3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (ball attachment abutment)	94	58147	PS TPA SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	82
58122	PS BA GH5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (ball attachment abutment)	94	58148	PS TPA SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment)	82

**Note:** Manufacturer notes about trade names, see page 125.

\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58150	PS HP, Ø4.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	32	58202	PS HPW, Ø6.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	33
58151	PS HP, Ø5.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	32	58203	PS HPW, Ø6.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	33
58152	PS HP, Ø5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	32	58204	PS HPW, Ø6.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	33
58153	PS HP, Ø6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	32	58205	PS HPW, Ø6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	33
58160	BEGO Semados® implant, SC 3.25 L8.5	22	58206	PS HPW, Ø7.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	33
58161	BEGO Semados® implant, SC 3.25 L10	22	58219	ST PMB, Ø16, S/RI 3.25–5.5 (milling blank)	99
58162	BEGO Semados® implant, SC 3.25 L11.5	22	58221	PS PMB, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (TI-Form milling blank)	78
58163	BEGO Semados® implant, SC 3.25 L13	22	58226	PS PMB, Ø16, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (milling blank)	78
58164	BEGO Semados® implant, SC 3.25 L15	22	58242	BEGO Semados® SCX implant large-scale model	124
58165	BEGO Semados® implant, SC 3.75 L8.5	22	58243	Maxilla demonstration model, SCX implants	125
58166	BEGO Semados® implant, SC 3.75 L10	22	58244	BEGO Semados® SC demo implants	125
58167	BEGO Semados® implant, SC 3.75 L11.5	22	58245	BEGO Semados® SCX demo implants	125
58168	BEGO Semados® implant, SC 3.75 L13	22	58246	Radiographic template, SC/SCX implants	20
58169	BEGO Semados® implant, SC 3.75 L15	22	58247	PS AS (selection set)	85
58170	BEGO Semados® implant, SC 4.1 L7	22	58250	PS CADP, RS/RSX 3.0 (CAD positioner)	76
58171	BEGO Semados® implant, SC 4.1 L8.5	22	58251	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (CAD positioner)	77
58172	BEGO Semados® implant, SC 4.1 L10	22	58252	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (CAD positioner)	77
58173	BEGO Semados® implant, SC 4.1 L11.5	22	58253	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (CAD positioner)	77
58174	BEGO Semados® implant, SC 4.1 L13	22	58254	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (CAD positioner)	77
58175	BEGO Semados® implant, SC 4.1 L15	22	58255	CADP MultiPlus (CAD positioner)	91, 109
58176	BEGO Semados® implant, SC 4.5 L7	22	58256	CADP, Mini (CAD positioner)	116
58177	BEGO Semados® implant, SC 4.5 L8.5	22	58260	BEGO Semados® implant, SCX 3.25 L8.5	23
58178	BEGO Semados® implant, SC 4.5 L10	22	58261	BEGO Semados® implant, SCX 3.25 L10	23
58179	BEGO Semados® implant, SC 4.5 L11.5	22	58262	BEGO Semados® implant, SCX 3.25 L11.5	23
58180	BEGO Semados® implant, SC 4.5 L13	22	58263	BEGO Semados® implant, SCX 3.25 L13	23
58181	BEGO Semados® implant, SC 4.5 L15	22	58264	BEGO Semados® implant, SCX 3.25 L15	23
58182	BEGO Semados® implant, SC 5.5 L7	22	58265	BEGO Semados® implant, SCX 3.75 L8.5	23
58183	BEGO Semados® implant, SC 5.5 L8.5	22	58266	BEGO Semados® implant, SCX 3.75 L10	23
58184	BEGO Semados® implant, SC 5.5 L10	22	58267	BEGO Semados® implant, SCX 3.75 L11.5	23
58185	BEGO Semados® implant, SC 5.5 L11.5	22	58268	BEGO Semados® implant, SCX 3.75 L13	23
58186	BEGO Semados® implant, SC 5.5 L13	22	58269	BEGO Semados® implant, SCX 3.75 L15	23
58191	CAD SP, S/SC/SCX/RS/RSX/RI 3.25–3.75 (scansupport)	77, 99	58270	BEGO Semados® implant, SCX 4.1 L7	23
58192	CAD SP, S/SC/SCX/RS/RSX/RI 4.1 (scansupport)	77, 99	58271	BEGO Semados® implant, SCX 4.1 L8.5	23
58193	CAD SP, S/SC/SCX/RS/RSX/RI 4.5 (scansupport)	77, 99	58272	BEGO Semados® implant, SCX 4.1 L10	23
58194	CAD SP, S/SC/SCX/RS/RSX/RI 5.5 (scansupport)	77, 99	58273	BEGO Semados® implant, SCX 4.1 L11.5	23
58200	PS HPW, Ø5.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	33			
58201	PS HPW, Ø5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	33			

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58274	BEGO Semados® implant, SCX 4.1 L13	23	58350	BEGO Semados® Tray <sup>Plus</sup> (empty), RS/RSX 3.0–5.5	57
58275	BEGO Semados® implant, SCX 4.1 L15	23	58351	BEGO Semados® Tray <sup>Plus</sup> (empty) S/SC/SCX 3.25–5.5	54
58276	BEGO Semados® implant, SCX 4.5 L7	23	58352	BEGO Semados® Tray <sup>Plus</sup> (empty), RI 3.75–5.5	60
58277	BEGO Semados® implant, SCX 4.5 L8.5	23	58353	Mini-/Osseodirect <sup>Plus</sup> Tray (empty), Mini 2.7–3.1	62
58278	BEGO Semados® implant, SCX 4.5 L10	23	58354	Drill stop Tray <sup>Plus</sup> (empty), S/SC/SCX	56
58279	BEGO Semados® implant, SCX 4.5 L11.5	23	58356	Drill stop Tray <sup>Plus</sup> (empty), RS/RSX	59
58280	BEGO Semados® implant, SCX 4.5 L13	23	58357	Prosthetic kit (empty)	66
58281	BEGO Semados® implant, SCX 4.5 L15	23	58370	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment)	77
58282	BEGO Semados® implant, SCX 5.5 L7	23	58371	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment)	77
58283	BEGO Semados® implant, SCX 5.5 L8.5	23	58372	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment)	77
58284	BEGO Semados® implant, SCX 5.5 L10	23	58373	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment)	77
58285	BEGO Semados® implant, SCX 5.5 L11.5	23	58374	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment no Hex)	78
58286	BEGO Semados® implant, SCX 5.5 L13	23	58375	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment no Hex)	78
58290	Implant cover screw, SC/SCX 3.25	32	58376	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment no Hex)	78
58297	PS OCP, GH 2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (restoration set)	79	58377	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment no Hex)	78
58298	PS OCP, GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (restoration set)	79	58386	BEGO Guide Tr (empty), RS/RSX 3.0–4.5	49
58299	PS OCP, GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (restoration set)	79	58387	BEGO Guide Tray (empty), S/SC/SCX 3.25–4.5	46
58300	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (restoration set)	79	58388	BEGO Semados® PI Tray (empty)	42
58301	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (restoration set)	79	58445	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.0 (bone shaper)	64
58302	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (restoration set)	79	58446	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (bone shapers)	64
58303	LCC (laboratory caps for crowns)	79	58447	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (bone shaper)	64
58304	LCB (laboratory caps for bridges)	79	58448	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (bone shaper)	64
58305	OCP A (implant analog)	79	58449	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (bone shaper)	64
58315	PS IMPA, SC/SCX 3.25 (implant analog)	80	58488	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12
58316	PS CTI, SC/SCX 3.25 (impression set, closed)	80	58489	naturesQue MaxOss P, 0.25–1.0mm 1.0ml	12
58317	PS OTI, SC/SCX 3.25 (impression set, open)	80	58490	naturesQue MaxOss P, 0.25–1.0mm 2.0ml	12
58319	ST PMB, Ø11.5, S/RI 3.25–5.5 (milling blank)	99	58491	naturesQue MaxOss P, 0.25–1.0mm 4.0ml	12
58322	BEGO Semados® RI* <sup>1</sup> implant large-scale model	124	58492	naturesQue MaxOss P, 1.0–2.0mm 1.0ml	12
58326	PS PMB, Ø11.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5(milling blank)	78	58493	naturesQue MaxOss P, 1.0–2.0mm 2.0ml	12
58345	BEGO Semados® RI* <sup>1</sup> demo implant	125			
58346	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> S/SC/SCX 3.75–4.5	54			
58347	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) S/SC/SCX 3.75–4.5	54			
58348	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> , RS/RSX 3.75–4.5	57			
58349	BEGO Semados®, Starter/Compact Tray <sup>Plus</sup> (empty), RS/RSX 3.75–4.5	57			

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page
58494	naturesQue MaxOss P, 0.25–1.0mm 0.25ml	12
58495	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12
58496	naturesQue ColTect P, 15 × 20mm	12
58497	naturesQue ColTect P, 20 × 30mm	12
58498	naturesQue ColTect P, 30 × 40mm	12
58499	naturesQue ColAid B, 0.1g	12
58500	naturesQue SemOss B, 0.25–1.0mm 0.5g; 1.0ml	12
58501	naturesQue SemOss B, 0.25–1.0mm 1.0g; 2.0ml	12
58502	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12
58503	naturesQue SemOss B, 0.25–1.0mm 2.0g; 4.0ml	12
58504	naturesQue SemOss B, 1.0–2.0mm 0.5g; 1.0ml	12
58505	naturesQue SemOss B, 1.0–2.0mm 1.0g; 2.0ml	12
58506	naturesQue SemOss B, 1.0–2.0mm 2.0g; 4.0ml	12
58507	naturesQue ColAid P, 20 × 20mm	12
83538	BEGO SECURITY Implants (implant warranty)	24, 30, 36, 40
549316	BEG 5.DIM, S/RI 3.25–3.75 (DIM-Analog®)	100
549317	BEG 5.DIM, S/RI 4.1 (DIM-Analog®)	100
549318	BEG 5.DIM, S/RI 4.5 (DIM analog®)	100
549319	BEG 5.DIM, S/RI 5.5 (DIM analog®)	100
549320	BEG 5.DIM, RS/RSX 3.0 (DIM-Analog®)	80
549321	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 3.25–3.75 (DIM-Analog®)	80
549322	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.1 (DIM-Analog®)	80
549323	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.5 (DIM analog®)	80
549324	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 5.5 (DIM analog®)	80
549528	BEG MU 5.DIM MultiPlus System (DIM-Analog®)	90, 108
549539	Screwdriver L24 (DYNAMIC® ABUTMENT)	71

## INDEX · PRODUCTS LISTED ALPHABETICALLY

<b>REF</b>	<b>Article</b>	<b>Page</b>
<b>A</b>		
56753	Acrylic block PS (large-scale model, scale 2:1)	<b>124</b>
55773	Activator/deactivator Dalbo®-PLUS	<b>94, 112, 120</b>
<b>B</b>		
55768	Ball attachment impression set Dalbo®-PLUS	<b>94, 112, 120</b>
56968	Ball attachment Mini, GH 1.5, Mini 2.9–3.1	<b>120</b>
57055	Ball attachment Mini, GH 4, Mini 2.9–3.1	<b>120</b>
549316	BEG 5.DIM, S/RI 3.25–3.75 (DIM-Analog®)	<b>100</b>
549317	BEG 5.DIM, S/RI 4.1 (DIM-Analog®)	<b>100</b>
549318	BEG 5.DIM, S/RI 4.5 (DIM-Analog®)	<b>100</b>
549319	BEG 5.DIM, S/RI 5.5 (DIM-Analog®)	<b>100</b>
549528	BEG MU 5.DIM Multi <sup>Plus</sup> System (DIM-Analog®)	<b>90, 108</b>
57221	BEGO Collagen Membrane, 15 × 20mm	<b>12</b>
57222	BEGO Collagen Membrane, 20 × 30mm	<b>12</b>
57223	BEGO Collagen Membrane, 30 × 40mm	<b>12</b>
58065	BEGO Guide Conn, with ratchet connection, Ø4.2 (AX), RS/RSX (connector)	<b>51</b>
58051	BEGO Guide CS, (3), RS/RSX 3.0 (countersink)	<b>50</b>
58052	BEGO Guide CS, (4), RS/RSX 3.75 (countersink)	<b>50</b>
58053	BEGO Guide CS, (5), RS/RSX 4.1 (countersink)	<b>50</b>
58054	BEGO Guide CS, (6), RS/RSX 4.5 (countersink)	<b>50</b>
58066	BEGO Guide Conn, with ratchet connection, Ø4.2 (AY), RS/RSX (connector)	<b>51</b>
58067	BEGO Guide Conn, with ratchet connection, Ø4.2 (AZ), RS/RSX (connector)	<b>51</b>
58068	BEGO Guide Conn, with ratchet connection, Ø4.7 (BX), RS/RSX (connector)	<b>51</b>
58069	BEGO Guide Conn, with ratchet connection, Ø4.7 (BY), RS/RSX (connector)	<b>51</b>
58070	BEGO Guide Conn, with ratchet connection, Ø4.7 (BZ), RS/RSX (connector)	<b>51</b>
58059	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AX), RS/RSX (connector)	<b>51</b>
58060	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AY), RS/RSX (connector)	<b>51</b>
58061	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AZ), RS/RSX (connector)	<b>51</b>
58062	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BX), RS/RSX (connector)	<b>51</b>
58063	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BY), RS/RSX (connector)	<b>51</b>
58064	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BZ), RS/RSX (connector)	<b>51</b>
57450	BEGO Guide spoon, Ø4.2 (AX), S/SC/SCX	<b>48</b>
57451	BEGO Guide spoon, Ø4.2 (AY), S/SC/SCX	<b>48</b>
57452	BEGO Guide spoon, Ø4.2 (AZ), S/SC/SCX	<b>48</b>
57453	BEGO Guide spoon, Ø4.7 (BX), S/SC/SCX	<b>48</b>

<b>REF</b>	<b>Article</b>	<b>Page</b>
57454	BEGO Guide spoon, Ø4.7 (BY), S/SC/SCX	<b>48</b>
57455	BEGO Guide spoon, Ø4.7 (BZ), S/SC/SCX	<b>48</b>
57713	BEGO Guide PD, Ø2.5 L18 (X2), RS/RSX (depth drill)	<b>50</b>
57714	BEGO Guide pilot drill, Ø2.5 L23.5 (Y2), RS/RSX (depth drill)	<b>50</b>
57715	BEGO Guide PD, Ø2.5 L29 (Z2), RS/RSX (depth drill)	<b>50</b>
57716	BEGO Guide DD, Ø2.8 L18 (X3), RS/RSX 3.0 (depth drill)	<b>50</b>
57717	BEGO Guide DD, Ø2.8 L23.5 (Y3), RS/RSX 3.0 (depth drill)	<b>50</b>
57723	BEGO Guide DD, Ø2.8 L29 (Z3), RS/RSX 3.0 (depth drill)	<b>50</b>
57724	BEGO Guide DD, Ø3.4 L18 (X4), RS/RSX 3.75 (depth drill)	<b>50</b>
57725	BEGO Guide DD, Ø3.4 L23.5 (Y4), RS/RSX 3.75 (depth drill)	<b>50</b>
57726	BEGO Guide DD, Ø3.4 L29 (Z4), RS/RSX 3.75 (depth drill)	<b>50</b>
57727	BEGO Guide DD, Ø3.8 L18 (X5), RS/RSX 4.1 (depth drill)	<b>50</b>
57733	BEGO Guide DD, Ø3.8 L23.5 (Y5), RS/RSX 4.1 (depth drill)	<b>50</b>
57734	BEGO Guide DD, Ø3.8 L29 (Z5), RS/RSX 4.1 (depth drill)	<b>50</b>
57735	BEGO Guide DD, Ø4.1 L18 (X6), RS/RSX 4.5 (depth drill)	<b>50</b>
57736	BEGO Guide DD, Ø4.1 L23.5 (Y6), RS/RSX 4.5 (depth drill)	<b>50</b>
57737	BEGO Guide DD, Ø4.1 L29 (Z6), RS/RSX 4.5 (depth drill)	<b>50</b>
57130	BEGO Guide DS (drill sleeves)	<b>52</b>
57421	BEGO Guide tissue punches, Ø4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	<b>46, 49</b>
57422	BEGO Guide tissue punches, Ø4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	<b>46, 49</b>
57446	BEGO Guide thread tap, (3), S/SC/SCX 3.25	<b>48</b>
57447	BEGO Guide thread tap, (4), S/SC/SCX 3.75	<b>48</b>
57448	BEGO Guide thread tap, (5), S/SC/SCX 4.1	<b>48</b>
57449	BEGO Guide thread tap, (6), S/SC/SCX 4.5	<b>48</b>
57442	BEGO Guide countersink, (3), S/SC/SCX 3.25	<b>47</b>
57443	BEGO Guide countersink, (4), S/SC/SCX 3.75	<b>47</b>
57444	BEGO Guide countersink, (5), S/SC/SCX 4.1	<b>47</b>
57445	BEGO Guide countersink, (6), S/SC/SCX 4.5	<b>47</b>
57395	BEGO Guide master sleeves, Ø4.2 (A), S/SC/SCX/RS/RSX	<b>46, 49</b>

**Note:** Manufacturer notes about trade names, see page 125.

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57397	BEGO Guide master sleeves, Ø 4.7 (B), S/SC/SCX/RS/RSX	46, 49	57416	BEGO Guide spoon, Ø 2.5 (B2), S/SC/SCX	46
57696	BEGO Guide PD, Ø 2.0 L18 (X1), RS/RSX (pilot drill)	50	57413	BEGO Guide spoon, Ø 2.8 (A3), S/SC/SCX 3.25	46
57697	BEGO Guide pilot drill, Ø 2.0 L23.5 (Y1), RS/RSX (pilot drill)	50	57417	BEGO Guide spoon, Ø 2.8 (B3), S/SC/SCX 3.25	46
57698	BEGO Guide PD, Ø 2.0 L29 (Z1), RS/RSX (pilot drill)	50	57414	BEGO Guide spoon, Ø 3.25 (A4), S/SC/SCX 3.75	46
57423	BEGO Guide pilot drill, Ø 1.6 L18 (X1), S/SC/SCX	47	57418	BEGO Guide spoon, Ø 3.25 (B4), S/SC/SCX 3.75	46
57424	BEGO Guide pilot drill, Ø 1.6 L23.5 (Y1), S/SC/SCX	47	57419	BEGO Guide spoon, Ø 3.65 (B5), S/SC/SCX 4.1	46
57425	BEGO Guide pilot drill, Ø 1.6 L29 (Z1), S/SC/SCX	47	57420	BEGO Guide spoon, Ø 4.0 (B6), S/SC/SCX 4.5	46
57458	BEGO Guide ratchet adapter for connector, S/SC/SCX	48	57426	BEGO Guide depth drill Ø 2.5, L18 (X2), S/SC/SCX	47
58055	BEGO Guide ST, (3), RS/RSX 3.0 (thread tap)	51	57427	BEGO Guide depth drill, Ø 2.5 L23.5 (Y2), S/SC/SCX	47
58056	BEGO Guide ST, (4), RS/RSX 3.75 (thread tap)	51	57428	BEGO Guide depth drill Ø 2.5, L29 (Z2), S/SC/SCX	47
58057	BEGO Guide ST, (5), RS/RSX 4.1 (thread tap)	51	57429	BEGO Guide depth drill Ø 2.8, L18 (X3), S/SC/SCX 3.25	47
57686	BEGO Guide Sp, Ø 2.0 (A1), RS/RSX (reduction sleeve)	49	57430	BEGO Guide depth drill Ø 2.8 L23.5 (Y3), S/SC/SCX 3.25	47
58058	BEGO Guide ST (6) RS/RSX 4.5 (thread tap)	51	57431	BEGO Guide depth drill Ø 2.8, L29 (Z3), S/SC/SCX 3.25	47
57690	BEGO Guide Sp, Ø 2.0 (B1), RS/RSX (reduction sleeve)	49	57432	BEGO Guide depth drill Ø 3.25, L18 (X4), S/SC/SCX 3.75	47
57687	BEGO Guide Sp, Ø 2.5 (A2), RS/RSX (reduction sleeve)	49	57433	BEGO Guide depth drill Ø 3.25 L23.5 (Y4), S/SC/SCX 3.75	47
57691	BEGO Guide Sp, Ø 2.5 (B2), RS/RSX (reduction sleeve)	49	57434	BEGO Guide depth drill Ø 3.25, L29 (Z4), S/SC/SCX 3.75	47
57688	BEGO Guide Sp, Ø 2.8 (A3), RS/RSX 3.0 (reduction sleeve)	49	57435	BEGO Guide depth drill Ø 3.65, L18 (X5), S/SC/SCX 4.1	47
57692	BEGO Guide Sp, Ø 2.8 (B3), RS/RSX 3.0 (reduction sleeve)	49	57436	BEGO Guide depth drill Ø 3.65 L23.5 (Y5), S/SC/SCX 4.1	47
57689	BEGO Guide Sp, Ø 3.4 (A4), RS/RSX 3.75 (reduction sleeve)	49	57437	BEGO Guide depth drill Ø 3.65, L29 (Z5), S/SC/SCX 4.1	47
57693	BEGO Guide Sp, Ø 3.4 (B4), RS/RSX 3.75 (reduction sleeve)	49	57438	BEGO Guide depth drill Ø 4.0, L18 (X6), S/SC/SCX 4.5	47
57694	BEGO Guide Sp, Ø 3.8 (B5), RS/RSX 4.1 (reduction sleeve)	49	57439	BEGO Guide depth drill Ø 4.0 L23.5 (Y6), S/SC/SCX 4.5	47
57695	BEGO Guide Sp, Ø 4.1 (B6), RS/RSX 4.5 (reduction sleeve)	49	57441	BEGO Guide depth drill Ø 4.0, L29 (Z6), S/SC/SCX 4.5	47
57411	BEGO Guide spoon, Ø 1.6 (A1), S/SC/SCX	46	57456	BEGO Guide depth stop ring connector, Ø 4.2 (A), S/SC/SCX/RS/RSX	48, 51
57415	BEGO Guide spoon, Ø 1.6 (B1), S/SC/SCX	46	57457	BEGO Guide depth stop ring connector, Ø 4.7 (B), S/SC/SCX/RS/RSX	48, 51
57412	BEGO Guide spoon, Ø 2.5 (A2), S/SC/SCX	46			

INDEX · PRODUCTS LISTED ALPHABETICALLY

## INDEX · PRODUCTS LISTED ALPHABETICALLY

<b>REF</b>	<b>Article</b>	<b>Page</b>
58386	BEGO Guide Tr (empty), RS/RSX 3.0–4.5	49
58071	BEGO Guide Tr, RS/RSX 3.0–4.5 (surgical tray)	49
58387	BEGO Guide Tray (empty), S/SC/SCX 3.25–4.5	46
57399	BEGO Guide Tray, S/SC/SCX 3.25–4.5	46
57459	BEGO Guide center drill, Ø 4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	47, 50
57463	BEGO Guide center drill, Ø 4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	47, 50
57400	BEGO Guide – pilot drill, short	52
57401	BEGO Guide – pilot drill, long	52
83538	BEGO SECURITY Implants (implant warranty)	24, 30, 36, 40
56750	BEGO Semados® RSX implant large-scale model	124
56947	BEGO Semados® implant, Mini 2.7 L11.5	40
56948	BEGO Semados® implant, Mini 2.7 L13	40
56949	BEGO Semados® implant, Mini 2.7 L15	40
56950	BEGO Semados® implant, Mini 2.9 L11.5	40
56951	BEGO Semados® implant, Mini 2.9 L13	40
56952	BEGO Semados® implant, Mini 2.9 L15	40
56953	BEGO Semados® implant, Mini 3.1 L11.5	40
56954	BEGO Semados® implant, Mini 3.1 L13	40
56955	BEGO Semados® implant, Mini 3.1 L15	40
57708	BEGO Semados® implant, RI 3.75 L8.5	30
57709	BEGO Semados® implant, RI 3.75 L10	30
57710	BEGO Semados® implant, RI 3.75 L11.5	30
57711	BEGO Semados® implant, RI 3.75 L13	30
57718	BEGO Semados® implant, RI 4.1 L8.5	30
57719	BEGO Semados® implant, RI 4.1 L10	30
57720	BEGO Semados® implant, RI 4.1 L11.5	30
57721	BEGO Semados® implant, RI 4.1 L13	30
57728	BEGO Semados® implant, RI 4.5 L8.5	30
57729	BEGO Semados® implant, RI 4.5 L10	30
57730	BEGO Semados® implant, RI 4.5 L11.5	30
57731	BEGO Semados® implant, RI 4.5 L13	30
57738	BEGO Semados® implant, RI 5.5 L8.5	30
57739	BEGO Semados® implant, RI 5.5 L10	30
57740	BEGO Semados® implant, RI 5.5 L11.5	30
57741	BEGO Semados® implant, RI 5.5 L13	30
57962	BEGO Semados® implant, RS 3.0 L10	26
57963	BEGO Semados® implant, RS 3.0 L11.5	26
57964	BEGO Semados® implant, RS 3.0 L13	26
57966	BEGO Semados® implant, RS 3.75 L8.5	26
57967	BEGO Semados® implant, RS 3.75 L10	26
57968	BEGO Semados® implant, RS 3.75 L11.5	26
57969	BEGO Semados® implant, RS 3.75 L13	26
57970	BEGO Semados® implant, RS 3.75 L15	26
57971	BEGO Semados® implant, RS 4.1 L7	26

<b>REF</b>	<b>Article</b>	<b>Page</b>
57972	BEGO Semados® implant, RS 4.1 L8.5	26
57973	BEGO Semados® implant, RS 4.1 L10	26
57974	BEGO Semados® implant, RS 4.1 L11.5	26
57975	BEGO Semados® implant, RS 4.1 L13	26
57976	BEGO Semados® implant, RS 4.1 L15	26
57977	BEGO Semados® implant, RS 4.5 L7	26
57978	BEGO Semados® implant, RS 4.5 L8.5	26
57979	BEGO Semados® implant, RS 4.5 L10	26
57980	BEGO Semados® implant, RS 4.5 L11.5	26
57981	BEGO Semados® implant, RS 4.5 L13	26
57982	BEGO Semados® implant, RS 4.5 L15	26
57983	BEGO Semados® implant, RS 5.5 L7	26
57984	BEGO Semados® implant, RS 5.5 L8.5	26
57985	BEGO Semados® implant, RS 5.5 L10	26
57986	BEGO Semados® implant, RS 5.5 L11.5	26
57987	BEGO Semados® implant, RS 5.5 L13	26
57862	BEGO Semados® implant, RSX 3.0 L10	27
57863	BEGO Semados® implant, RSX 3.0 L11.5	27
57864	BEGO Semados® implant, RSX 3.0 L13	27
57866	BEGO Semados® implant, RSX 3.75 L8.5	27
57867	BEGO Semados® implant, RSX 3.75 L10	27
57868	BEGO Semados® implant, RSX 3.75 L11.5	27
57869	BEGO Semados® implant, RSX 3.75 L13	27
57870	BEGO Semados® implant, RSX 3.75 L15	27
57871	BEGO Semados® implant, RSX 4.1 L7	27
57872	BEGO Semados® implant, RSX 4.1 L8.5	27
57873	BEGO Semados® implant, RSX 4.1 L10	27
57874	BEGO Semados® implant, RSX 4.1 L11.5	27
57875	BEGO Semados® implant, RSX 4.1 L13	27
57876	BEGO Semados® implant, RSX 4.1 L15	27
57877	BEGO Semados® implant, RSX 4.5 L7	27
57878	BEGO Semados® implant, RSX 4.5 L8.5	27
57879	BEGO Semados® implant, RSX 4.5 L10	27
57880	BEGO Semados® implant, RSX 4.5 L11.5	27
57881	BEGO Semados® implant, RSX 4.5 L13	27
57882	BEGO Semados® implant, RSX 4.5 L15	27
57883	BEGO Semados® implant, RSX 5.5 L7	27
57884	BEGO Semados® implant, RSX 5.5 L8.5	27
57885	BEGO Semados® implant, RSX 5.5 L10	27
57886	BEGO Semados® implant, RSX 5.5 L11.5	27
57887	BEGO Semados® implant, RSX 5.5 L13	27
57500	BEGO Semados® implant, S 3.25 L8.5	36
57501	BEGO Semados® implant, S 3.25 L10	36
57502	BEGO Semados® implant, S 3.25 L11.5	36
57503	BEGO Semados® implant, S 3.25 L13	36
57601	BEGO Semados® implant, S 3.75 L8.5	36
57602	BEGO Semados® implant, S 3.75 L10	36

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

# INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57603	BEGO Semados® implant, S 3.75 L11.5	36	58264	BEGO Semados® implant, SCX 3.25 L15	23
57604	BEGO Semados® implant, S 3.75 L13	36	58265	BEGO Semados® implant, SCX 3.75 L8.5	23
57840	BEGO Semados® implant, S 4.1 L7	36	58266	BEGO Semados® implant, SCX 3.75 L10	23
57841	BEGO Semados® implant, S 4.1 L8.5	36	58267	BEGO Semados® implant, SCX 3.75 L11.5	23
57842	BEGO Semados® implant, S 4.1 L10	36	58268	BEGO Semados® implant, SCX 3.75 L13	23
57843	BEGO Semados® implant, S 4.1 L11.5	36	58269	BEGO Semados® implant, SCX 3.75 L15	23
57844	BEGO Semados® implant, S 4.1 L13	36	58270	BEGO Semados® implant, SCX 4.1 L7	23
57700	BEGO Semados® implant, S 4.5 L7	36	58271	BEGO Semados® implant, SCX 4.1 L8.5	23
57701	BEGO Semados® implant, S 4.5 L8.5	36	58272	BEGO Semados® implant, SCX 4.1 L10	23
57702	BEGO Semados® implant, S 4.5 L10	36	58273	BEGO Semados® implant, SCX 4.1 L11.5	23
57703	BEGO Semados® implant, S 4.5 L11.5	36	58274	BEGO Semados® implant, SCX 4.1 L13	23
57704	BEGO Semados® implant, S 4.5 L13	36	58275	BEGO Semados® implant, SCX 4.1 L15	23
57901	BEGO Semados® implant, S 5.5 L8.5	36	58276	BEGO Semados® implant, SCX 4.5 L7	23
57902	BEGO Semados® implant, S 5.5 L10	36	58277	BEGO Semados® implant, SCX 4.5 L8.5	23
57903	BEGO Semados® implant, S 5.5 L11.5	36	58278	BEGO Semados® implant, SCX 4.5 L10	23
57904	BEGO Semados® implant, S 5.5 L13	36	58279	BEGO Semados® implant, SCX 4.5 L11.5	23
58160	BEGO Semados® implant, SC 3.25 L8.5	22	58280	BEGO Semados® implant, SCX 4.5 L13	23
58161	BEGO Semados® implant, SC 3.25 L10	22	58281	BEGO Semados® implant, SCX 4.5 L15	23
58162	BEGO Semados® implant, SC 3.25 L11.5	22	58282	BEGO Semados® implant, SCX 5.5 L7	23
58163	BEGO Semados® implant, SC 3.25 L13	22	58283	BEGO Semados® implant, SCX 5.5 L8.5	23
58164	BEGO Semados® implant, SC 3.25 L15	22	58284	BEGO Semados® implant, SCX 5.5 L10	23
58165	BEGO Semados® implant, SC 3.75 L8.5	22	58285	BEGO Semados® implant, SCX 5.5 L11.5	23
58166	BEGO Semados® implant, SC 3.75 L10	22	58286	BEGO Semados® implant, SCX 5.5 L13	23
58167	BEGO Semados® implant, SC 3.75 L11.5	22	55709	BEGO Semados® Mini demo implants	125
58168	BEGO Semados® implant, SC 3.75 L13	22	57095	BEGO Semados® Mini implant large-scale model	124
58169	BEGO Semados® implant, SC 3.75 L15	22	57670	BEGO Semados® PI tray	42
58170	BEGO Semados® implant, SC 4.1 L7	22	58388	BEGO Semados® PI Tray (empty)	42
58171	BEGO Semados® implant, SC 4.1 L8.5	22	57660	BEGO Semados® Provisional Implant (PI), 1 unit	42
58172	BEGO Semados® implant, SC 4.1 L10	22	57673	BEGO Semados® Provisional Implant (PI), 10 units	42
58173	BEGO Semados® implant, SC 4.1 L11.5	22	55599	BEGO Semados® ratchet adapter	43, 64, 66
58174	BEGO Semados® implant, SC 4.1 L13	22	58345	BEGO Semados® RI*1 demo implant	125
58175	BEGO Semados® implant, SC 4.1 L15	22	58322	BEGO Semados® RI*1 implant large-scale model	124
58176	BEGO Semados® implant, SC 4.5 L7	22	56751	BEGO Semados® RS demo implants	125
58177	BEGO Semados® implant, SC 4.5 L8.5	22	56752	BEGO Semados® RSX demo implants	125
58178	BEGO Semados® implant, SC 4.5 L10	22	58699	BEGO Semados® RSX demo implants 3.0	125
58179	BEGO Semados® implant, SC 4.5 L11.5	22	55543	BEGO Semados® S demo implants	125
58180	BEGO Semados® implant, SC 4.5 L13	22	58244	BEGO Semados® SC demo implants	125
58181	BEGO Semados® implant, SC 4.5 L15	22	58245	BEGO Semados® SCX demo implants	125
58182	BEGO Semados® implant, SC 5.5 L7	22	58242	BEGO Semados® SCX implant large-scale model	124
58183	BEGO Semados® implant, SC 5.5 L8.5	22	58346	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> S/SC/SCX 3.75–4.5	54
58184	BEGO Semados® implant, SC 5.5 L10	22	58347	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) S/SC/SCX 3.75–4.5	54
58185	BEGO Semados® implant, SC 5.5 L11.5	22	58351	BEGO Semados® Tray <sup>Plus</sup> (empty) S/SC/SCX 3.25–5.5	54
58186	BEGO Semados® implant, SC 5.5 L13	22			
58260	BEGO Semados® implant, SCX 3.25 L8.5	23			
58261	BEGO Semados® implant, SCX 3.25 L10	23			
58262	BEGO Semados® implant, SCX 3.25 L11.5	23			
58263	BEGO Semados® implant, SCX 3.25 L13	23			

# INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58352	BEGO Semados® Tray <sup>Plus</sup> (empty), RI 3.75–5.5	60	57487	DD D1, RS/RSX 4.5 (depth drill)	58
58350	BEGO Semados® Tray <sup>Plus</sup> (empty), RS/RSX 3.0–5.5	57	57488	DD D1, RS/RSX 5.5 (depth drill)	58
57340	BEGO Semados® Tray <sup>Plus</sup> , S/SC/SCX 3.25–5.5	54	57995	DD, Mini 2.7 (depth drill)	62
57612	BEGO Semados® Tray <sup>Plus</sup> , RI 3.75–5.5	60	57996	DD, Mini 2.9 (depth drill)	62
57949	BEGO Semados® Tray <sup>Plus</sup> , RS/RSX 3.0–5.5	57	57997	DD, Mini 3.1 (depth drill)	62
58349	BEGO Semados®, Starter/Compact Tray <sup>Plus</sup> (empty), RS/RSX 3.75–4.5	57	57926	Depth drill 2.5 short, RS/RSX	57
58348	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> , RS/RSX 3.75–4.5	57	57100	Depth drill 2.5 short, S/SC/SCX	55
549320	BEG 5.DIM, RS/RSX 3.0 (DIM-Analog®)	80	57927	Depth drill 2.5 long, RS/RSX	57
549321	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 3.25–3.75 (DIM-Analog®)	80	57101	Depth drill 2.5 long, S/SC/SCX	55
549322	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.1 (DIM-Analog®)	80	57583	Depth drill 3.2 short, RI	60
549323	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.5 (DIM-Analog®)	80	57584	Depth drill 3.2 long, RI	60
549324	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 5.5 (DIM-Analog®)	80	57585	Depth drill short, RI 3.75	61
<b>C</b>					
58191	CAD SP, S/SC/SCX/RS/RSX/RI 3.25–3.75 (scansupport)	77, 99	57587	Depth drill short, RI 4.1	61
58192	CAD SP, S/SC/SCX/RS/RSX/RI 4.1 (scansupport)	77, 99	57589	Depth drill short, RI 4.5	61
58193	CAD SP, S/SC/SCX/RS/RSX/RI 4.5 (scansupport)	77, 99	57591	Depth drill short, RI 5.5	61
58194	CAD SP, S/SC/SCX/RS/RSX/RI 5.5 (scansupport)	77, 99	57928	Depth drill short, RS/RSX 3.0	58
58255	CADP Multi <sup>Plus</sup> (CAD positioner)	91, 109	57930	Depth drill short, RS/RSX 3.75	58
58256	CADP, Mini (CAD positioner)	116	57932	Depth drill short, RS/RSX 4.1	58
57592	Countersink, RI 3.75	61	57934	Depth drill short, RS/RSX 4.5	58
57593	Countersink, RI 4.1	61	57936	Depth drill short, RS/RSX 5.5	58
57594	Countersink, RI 4.5	61	57102	Depth drill short, S/SC/SCX 3.25	55
57595	Countersink, RI 5.5	61	57104	Depth drill short, S/SC/SCX 3.75	55
57937	Countersink, RS/RSX 3.0	58	57106	Depth drill short, S/SC/SCX 4.1	55
57938	Countersink, RS/RSX 3.75	58	57108	Depth drill short, S/SC/SCX 4.5	55
57939	Countersink, RS/RSX 4.1	58	57110	Depth drill short, S/SC/SCX 5.5	55
57940	Countersink, RS/RSX 4.5	58	57586	Depth drill long, RI 3.75	61
57941	Countersink, RS/RSX 5.5	58	57588	Depth drill long, RI 4.1	61
57350	Countersink, S/SC/SCX 3.25	55	57590	Depth drill long, RI 4.5	61
57351	Countersink, S/SC/SCX 3.75	55	57929	Depth drill long, RS/RSX 3.0	58
57352	Countersink, S/SC/SCX 4.1	55	57931	Depth drill long, RS/RSX 3.75	58
57353	Countersink, S/SC/SCX 4.5	55	57933	Depth drill long, RS/RSX 4.1	58
57354	Countersink, S/SC/SCX 5.5	55	57935	Depth drill long, RS/RSX 4.5	58
<b>D</b>					
57484	DD D1, RS/RSX 3.0 (depth drill)	58	57103	Depth drill long, S/SC/SCX 3.25	55
57485	DD D1, RS/RSX 3.75 (depth drill)	58	57105	Depth drill long, S/SC/SCX 3.75	55
57486	DD D1, RS/RSX 4.1 (depth drill)	58	57107	Depth drill long, S/SC/SCX 4.1	55
<b>Note:</b> Manufacturer notes about trade names, see page 125.					
*1 New version of the BEGO Semados® RI implants, with Platform Switch design					
156					

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57476	Drill stops for depth drill 2.5 RS/RSX	59	56304	Healing abutment, Ø6.0 L5, S/RI 3.25-5.5	38
57477	Drill stops, RS/RSX 3.0	59	56305	Healing abutment, Ø6.0 L7, S/RI 3.25-5.5	38
57478	Drill stops, RS/RSX 3.75	59	53949	Hexagon screwdriver 1.25mm, short, with ratchet connection	66
57479	Drill stops, RS/RSX 4.1–4.5	59	55563	Hexagon screwdriver 1.25mm, short, contra-angle	66
57480	Drill stops, RS/RSX 5.5	59	53948	Hexagon screwdriver 1.25mm, long, with ratchet connection	66
55715	Drill stops, S/SC/SCX 4.1	56	55564	Hexagon screwdriver 1.25mm, long, contra-angle	66
55810	Drill stops, S/SC/SCX 4.5	56	57266	Hexagon screwdriver 1.25mm XS, with ratchet connection	66
55910	Drill stops, S/SC/SCX 5.5	56	I		
55804	Drill stops, depth drill 2.5 and S/SC/SCX 3.25–3.75	56	56749	IDC, RS/RSX 3.0 (adjustment instrument)	63
<b>E</b>			56748	IDC, S/SC/SCX/RS/RSX/RI 3.25–5.5 (adjustment instrument)	63
57751	Easy-Con impression coping	92, 110, 118	56956	Implant cover screw Mini	40
57760	Easy-Con analog	92, 110, 118	57950	Implant cover screw, RS/RSX 3.0	32
57754	Easy-Con production insert (black)	93, 111, 119	55505	Implant cover screw, S 3.25	38
57753	Easy-Con instrument	93, 111, 119	58290	Implant cover screw, SC/SCX 3.25	32
57752	Easy-Con laboratory set	93, 111, 119	57951	Implant cover screw, SC/SCX/RS/RSX/RI*1 3.75	32
57623	Easy-Con Mini, L1.5, Mini 3.1	118	57952	Implant cover screw, SC/SCX/RS/RSX/RI*1 4.1	32
57624	Easy-Con Mini, L2.5, Mini 3.1	118	57953	Implant cover screw, SC/SCX/RS/RSX/RI*1 4.5	32
57625	Easy-Con Mini, L3.5, Mini 3.1	118	57954	Implant cover screw, SC/SCX/RS/RSX/RI*1 5.5	32
57755	Easy-Con retention insert (blue)	93, 111, 119	55608	Implant cover screw, S/RI 3.75	38
57759	Easy-Con retention insert (green)	93, 111, 119	55615	Implant cover screw, S/RI 4.1	38
57757	Easy-Con retention insert (transparent)	93, 111, 119	55616	Implant cover screw, S/RI 4.5	38
57756	Easy-Con retention insert (pink)	93, 111, 119	55908	Implant cover screw, S/RI 5.5	38
57758	Easy-Con retention insert (red)	93, 111, 119	55714	Initial drill, Mini implants	62
57539	External reamer Multi <sup>Plus</sup>	91, 109	57533	Insertion instrument Multi <sup>Plus</sup> abutment 0°	88, 106
55537	External reamer Universal	86, 104	57008	Insert tool Easy-Con/Locator®	92, 110, 118
<b>F</b>			55831	Insert tool for implants, short, with ratchet connection	63
55769	Female parts Dalbo®-PLUS	94, 112, 120	56990	Insert tool for implants, short, with contra-angle connection	63
<b>G</b>			55830	Insert tool for implants, long, with ratchet connection	63
57320	Gold cast-on Mini, Mini 2.9–3.1	117	55832	Insert tool for implants, long, with contra-angle connection	63
53897	Guiding wrench	63	55880	Insert tool for ball attachment	94, 112, 120
<b>H</b>			57323	Internal reamer for gold cast-on Mini	117
55953	Healing abutment, individual Ø7, S/SC/SCX/RS/RSX/RI 3.25–5.5	33, 38	53735	Internal reamer for gold cast-on abutment	87, 105
56957	Healing abutment Mini, Ø3.5 L3, Mini 2.7–3.1	40	57540	Internal reamer Multi <sup>Plus</sup>	91, 109
56958	Healing abutment Mini, Ø3.5 L4, Mini 2.7–3.1	40	55536	Internal reamer Universal	86, 104
57252	Healing abutment Mini, Ø3.5 L7, Mini 2.7–3.1	40			
57324	Healing abutment, conical, S/RI 3.25–3.75	38			
55590	Healing abutment, Ø4.0 L3, S/RI 3.25–3.75	38			
55591	Healing abutment, Ø4.0 L5, S/RI 3.25–3.75	38			
55592	Healing abutment, Ø4.0 L7, S/RI 3.25–3.75	38			
56300	Healing abutment, Ø4.5 L3, S/RI 3.25–4.5	38			
56301	Healing abutment, Ø4.5 L5, S/RI 3.25–4.5	38			
56302	Healing abutment, Ø4.5 L7, S/RI 3.25–4.5	38			
55593	Healing abutment, Ø5.0 L3, S/RI 3.25–4.5	38			
55594	Healing abutment, Ø5.0 L5, S/RI 3.25–4.5	38			
55595	Healing abutment, Ø5.0 L7, S/RI 3.25–4.5	38			
56303	Healing abutment, Ø6.0 L3, S/RI 3.25–5.5	38			

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page
<b>L</b>		
58304	LCB (laboratory caps for bridges)	79
58303	LCC (laboratory caps for crowns)	79
<b>M</b>		
56755	Maxilla demonstration model, RSX implants	125
58243	Maxilla demonstration model, SCX implants	125
58353	Mini-/Osseo <sup>Plus</sup> Tray (empty), Mini 2.7–3.1	62
56970	Mini-/Osseo <sup>Plus</sup> Tray, Mini 2.7–3.1	62
56982	Model implant Mini	116
56694	Model implant, 3.25	100
56695	Model implant, S/RI 3.75	100
56696	Model implant, S/RI 4.1	100
56698	Model implant, S/RI 4.5	100
56699	Model implant, S/RI 5.5	100
57530	Multi <sup>Plus</sup> alignment aid, 20°	88, 106
57531	Multi <sup>Plus</sup> alignment aid, 30°	88, 106
57532	Multi <sup>Plus</sup> insertion splint	88, 106
57520	Multi <sup>Plus</sup> healing post	89, 107
57521	Multi <sup>Plus</sup> healing post, Mushroom	89, 107
57522	Multi <sup>Plus</sup> closed-tray impression, short	90, 108
57554	Multi <sup>Plus</sup> closed-tray impression, long	90, 108
57524	Multi <sup>Plus</sup> implant analog, 1 unit	90, 108
57525	Multi <sup>Plus</sup> implant analog, 4 units	90, 108
57523	Multi <sup>Plus</sup> open-tray impression	90, 108
57526	Multi <sup>Plus</sup> titanium abutment	91, 109
57538	Multi <sup>Plus</sup> Universal	91, 109
<b>N</b>		
58499	naturesQue ColAid B, 0.1g	12
58507	naturesQue ColAid P, 20 × 20mm	12
58496	naturesQue ColTect P, 15 × 20mm	12
58497	naturesQue ColTect P, 20 × 30mm	12
58498	naturesQue ColTect P, 30 × 40mm	12
58494	naturesQue MaxOss P, 0.25–1.0mm 0.25ml	12
58495	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12
58488	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12
58489	naturesQue MaxOss P, 0.25–1.0mm 1.0ml	12
58490	naturesQue MaxOss P, 0.25–1.0mm 2.0ml	12
58491	naturesQue MaxOss P, 0.25–1.0mm 4.0ml	12
58492	naturesQue MaxOss P, 1.0–2.0mm 1.0ml	12
58493	naturesQue MaxOss P, 1.0–2.0mm 2.0ml	12
58500	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12
58501	naturesQue SemOss B, 0.25–1.0mm 1.0g; 2.0ml	12
58502	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12
<b>O</b>		
58503	naturesQue SemOss B, 0.25–1.0mm 2.0g; 4.0ml	12
58504	naturesQue SemOss B, 1.0–2.0mm 0.5g; 1.0ml	12
58505	naturesQue SemOss B, 1.0–2.0mm 1.0g; 2.0ml	12
58506	naturesQue SemOss B, 1.0–2.0mm 2.0g; 4.0ml	12
<b>P</b>		
56972	Paralleling post, Mini	63
57598	Paralleling post, RI	63
57956	Paralleling post, RS/RSX	63
55863	Paralleling post, S/SC/SCX	63
57666	PI removal tool	43
57667	PI bending instrument	43
57665	PI insert tool	43
57671	PI implant analog	42
57661	PI multifunctional cap, 1 unit	42
57674	PI multifunctional cap, 5 unit	42
57663	PI paralleling post	43
57668	PI ratchet	43
57662	PI protection cap	42
57669	PI stabilizer	43
57664	PI depth drill	43
57581	Pilot marker, short, RI	60
57481	Pilot marker, short, RS/RSX	57
57308	Pilot marker, short, S/SC/SCX	54
57582	Pilot marker, long, RI	60
57482	Pilot marker, long, RS/RSX	57
57309	Pilot marker, long, S/SC/SCX	54
55826	Prosthetic kit	66
58357	Prosthetic kit (empty)	66
53999	Prosthesis screw Hex 1.25mm	95, 113
56983	Prosthesis screw Mini	121
57321	Prosthesis screw Mini, conical	121
55534	Prosthesis screw Sub-Tec Universal, S/RI 3.25–4.5	113
55535	Prosthesis screw Sub-Tec Universal, S/RI 5.5	113
57031	Prosthesis screw Sub-Tec <sup>Plus</sup>	95, 113
58247	PS AS (selection set)	85
58120	PS BA, GHO, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	94
58123	PS BA, GHO, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	94

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58126	PS BA, GH0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	94	58138	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	92
58121	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	94	58131	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	92
58124	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	94	58135	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	92
58127	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	94	58139	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	92
58122	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	94	58142	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (abutment)	92
58125	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	94	58132	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	92
58128	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	94	58136	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	92
58445	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.0 (bone shaper)	64	58140	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	92
58446	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (bone shapers)	64	58133	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	92
58447	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (bone shaper)	64	58137	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	92
58448	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (bone shaper)	64	58141	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	92
58449	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (bone shaper)	64	58143	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (abutment)	92
58250	PS CADP, RS/RSX 3.0 (CAD positioner)	76	58096	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (gold cast-on abutment no Hex)	87
58251	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (CAD positioner)	77	58097	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (gold cast-on abutment no Hex)	87
58252	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (CAD positioner)	77	58098	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (gold cast-on abutment no Hex)	87
58253	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (CAD positioner)	77	58099	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (gold cast-on abutment no Hex)	87
58254	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (CAD positioner)	77	58092	PS GCO, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (gold cast-on abutment)	87
57773	PS CTI, SC/SCX 3.0 (impression set, closed)	80	58093	PS GCO SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (gold cast-on abutment)	87
58316	PS CTI, SC/SCX 3.25 (impression set, closed)	80	58094	PS GCO, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (gold cast-on abutment)	87
57799	PS CTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (impression set, closed)	80	57764	PS HP, Ø3.0 L3, RS/RSX 3.0 (healing abutment)	32
57800	PS CTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (impression set, closed)	80	57765	PS HP, Ø3.0 L5, RS/RSX 3.0 (healing abutment)	32
57801	PS CTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (impression set, closed)	80	57766	PS HP, Ø3.0 L7, RS/RSX 3.0 (healing abutment)	32
57802	PS CTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (impression set, closed)	80	57767	PS HP, Ø4.0 L3, RS/RSX 3.0 (healing abutment)	32
58130	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	92	57768	PS HP, Ø4.0 L5, RS/RSX 3.0 (healing abutment)	32
58134	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	92	57769	PS HP, Ø4.0 L7, RS/RSX 3.0 (healing abutment)	32
			57807	PS HP, Ø4.5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	32

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57808	PS HP, Ø4.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	32	57819	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (implant analog)	80
58150	PS HP, Ø4.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	32	57820	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (implant analog)	80
57809	PS HP, Ø5.0 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	32	57821	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (implant analog)	80
57810	PS HP, Ø5.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	32	57822	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (implant analog)	80
58151	PS HP, Ø5.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	32	57778	PS ITA, RS/RSX 3.0 (temporary abutment)	81
57811	PS HP, Ø5.5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	32	58076	PS ITA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	82
57812	PS HP, Ø5.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	32	58077	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	82
58152	PS HP, Ø5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	32	58078	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	82
57813	PS HP, Ø6.5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	32	58100	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	88
57814	PS HP, Ø6.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	32	58102	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	88
58153	PS HP, Ø6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	32	58104	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	88
57815	PS HPW, Ø5.5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	33	58101	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	88
58200	PS HPW, Ø5.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	33	58103	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	88
58201	PS HPW, Ø5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	33	58105	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	88
57816	PS HPW, Ø6.0 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	33	58108	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	89
58202	PS HPW, Ø6.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	33	58110	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	89
58203	PS HPW, Ø6.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	33	58112	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	89
57817	PS HPW, Ø6.5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	33	58109	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	89
58204	PS HPW, Ø6.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	33	58111	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	89
58205	PS HPW, Ø6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	33	58113	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	89
57818	PS HPW, Ø7.0 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	33	58116	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	89
58206	PS HPW, Ø7.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	33	58117	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	89
57796	PS IMPA, RS/RSX 3.0 (implant analog)	80	58118	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	89
58315	PS IMPA, SC/SCX 3.25 (implant analog)	80	58297	PS OCP, GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (restoration set)	79

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58298	PS OCP, GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (restoration set)	79	57851	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	83
58299	PS OCP, GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (restoration set)	79	57853	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	83
58300	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (restoration set)	79	58088	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	83
58301	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (restoration set)	79	58089	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	83
58302	PS OCP, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (restoration set)	79	58090	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	83
57774	PS CTI, RS/RSX 3.0 (impression set, open)	80	58091	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	83
58317	PS OTI, SC/SCX 3.25 (impression set, open)	80	57891	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
57803	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (impression set, open)	80	57895	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
57804	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (impression set, open)	80	57899	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84
57805	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (impression set, open)	80	57907	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84
57806	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (impression set, open)	80	57798	PS TiAA, 15° E GH 2.5–4, RS/RSX 3.0 (solid abutment)	81
58221	PS PMB, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (TI-Form milling blank)	78	57892	PS TiAA, 15° E GH 2.5–4, SC/SCX/S/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
58326	PS PMB, Ø11.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5(milling blank)	78	57896	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
58226	PS PMB, Ø16, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (milling blank)	78	57900	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84
58072	PS PPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	82	57908	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84
58073	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	82	57889	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
58074	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	82	57893	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
58075	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment)	82	57897	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84
57846	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	83	57905	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	84
57848	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	83	57797	PS TiAA, 15° P GH 2.5–4, RS/RSX 3.0 (solid abutment)	81
57850	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	83	57890	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	84
57852	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	83	57894	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	84
57776	PS TiA, GH 2.5–4, RS/RSX 3.0 (solid abutment)	81	57898	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	84
57847	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	83			
57849	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	83			

## INDEX · PRODUCTS LISTED ALPHABETICALLY

<b>REF</b>	<b>Article</b>	<b>Page</b>	<b>REF</b>	<b>Article</b>	<b>Page</b>
57906	PS TiAA, 15° P GH 2.5-4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	84	58374	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI*1 3.25–3.75(adhesive abutment no Hex)	78
57911	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	85	58375	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment no Hex)	78
57915	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	85	58376	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment no Hex)	78
57919	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	85	58377	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment no Hex)	78
57923	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	85	57823	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment)	77
57912	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	85	57824	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment)	77
57916	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	85	57825	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment)	77
57920	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	85	57826	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment)	77
57924	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	85	58370	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment)	77
57909	PS TiAA, 20° P GH 1–2,SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	85	58371	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment)	77
57913	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	85	58372	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment)	77
57917	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	85	58373	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment)	77
57921	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	85	57781	PS TiB, RS/RSX 3.0 (adhesive abutment)	76
57910	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	85	58146	PS TPA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	82
57914	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	85	58147	PS TPA SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	82
57918	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	85	58148	PS TPA SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment)	82
57922	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	85	57858	PS TTiA NH, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment no Hex)	82
57827	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment no Hex)	78	57859	PS TTiA NH, SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment no Hex)	82
57828	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment no Hex)	78	57860	PS TTiA NH, SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment no Hex)	82
57829	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment no Hex)	78	57861	PS TTiA NH, SC/SCX/RS/RSX/RI*1 5.5 (temporary abutment no Hex)	82
57830	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment no Hex)	78	57854	PS TTiA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	82
			57855	PS TTiA, SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	82
			57856	PS TTiA, SC/SCX/RS/RSX/RI*1 4.5 (temporary abutment)	82
			57857	PS TTiA, SC/SCX/RS/RSX/RI*1 5.5 (temporary abutment)	82

**Note:** Manufacturer notes about trade names, see page 125.

\*1 New version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57835	PS UNI NH, SC/SCX/RS/RSX/RI*1 3.25–3.75 (Universal no Hex abutment)	86	57656	Sub-Tec CAD/CAM TiBase L, S/RI 3.25–3.75	99
57836	PS UNI NH, SC/SCX/RS/RSX/RI*1 4.1 (Universal abutment no Hex)	86	57657	Sub-Tec CAD/CAM TiBase L, S/RI 4.1	99
57837	PS UNI NH, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment no Hex)	86	57658	Sub-Tec CAD/CAM TiBase L, S/RI 4.5	99
57838	PS UNI NH, SC/SCX/RS/RSX/RI*1 5.5 (Universal abutment no Hex)	86	57659	Sub-Tec CAD/CAM TiBase L, S/RI 5.5	99
57993	PS UNI PScrew (prosthesis screw)	95	57286	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 3.25–3.75	98
57831	PS UNI, SC/SCX/RS/RSX/RI*1 3.25–3.75 (Universal abutment)	86	57288	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.1	98
57832	PS UNI, SC/SCX/RS/RSX/RI*1 4.1 (Universal abutment)	86	57290	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.5	98
57833	PS UNI, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment)	86	57292	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 5.5	98
57834	PS UNI, SC/SCX/RS/RSX/RI*1 5.5 (Universal abutment)	86	57285	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 3.25–3.75	98
57782	Pscrew (prosthesis screw Ø3.0)	95	57287	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.1	98
57784	Pscrew (prosthesis screw, for CAD positioner Ø3.0)	95	57289	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.5	98
<b>R</b>			57291	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 5.5	98
57010	Radiographic template, Mini implants	20	57743	Sub-Tec Easy-Con abutment, L1, S/RI 3.75–4.1	110
57672	Radiographic template, PI implants	20	57747	Sub-Tec Easy-Con abutment, L1, S/RI 4.5	110
55745	Radiographic template, RI implants	20	57744	Sub-Tec Easy-Con abutment, L2, S/RI 3.75–4.1	110
57959	Radiographic template, RS/RSX implants	20	57748	Sub-Tec Easy-Con abutment, L2, S/RI 4.5	110
53888	Radiographic template, S implants	20	57745	Sub-Tec Easy-Con abutment, L3, S/RI 3.75–4.1	110
58246	Radiographic template, SC/SCX implants	20	57749	Sub-Tec Easy-Con abutment, L3, S/RI 4.5	110
55799	Ratchet/torque wrench	64, 66	57746	Sub-Tec Easy-Con abutment, L4, S/RI 3.75–4.1	110
55776	Retention insert Dalbo®-PLUS	94, 112, 120	57750	Sub-Tec Easy-Con abutment, L4, S/RI 4.5	110
<b>S</b>			55873	Sub-Tec gold cast-on no Hex, S/RI 3.25–3.75	105
549539	Screwdriver L24 (DYNAMIC® ABUTMENT)	71	55625	Sub-Tec gold cast-on no Hex, S/RI 4.1	105
57535	Secondary screw Multi <sup>Plus</sup> (M1.8)	95, 113	56325	Sub-Tec gold cast-on no Hex, S/RI 4.5	105
57534	Secondary screw Multi <sup>Plus</sup> (M1.4)	95, 113	56515	Sub-Tec gold cast-on no Hex, S/RI 5.5	105
53952	Slot screwdriver, long with ratchet connection	66	55862	Sub-Tec gold cast-on, S/RI 3.25–3.75	105
58319	ST PMB, Ø11.5, S/RI 3.25–5.5 (milling blank)	99	55624	Sub-Tec gold cast-on, S/RI 4.1	105
58219	ST PMB, Ø16, S/RI 3.25–5.5 (milling blank)	99	56317	Sub-Tec gold cast-on, S/RI 4.5	105
55860	Sub-Dent closed-tray impression, S 3.25	100	57631	Sub-Tec ball attachment, GH 0, S/RI 3.25–3.75	112
55539	Sub-Dent closed-tray impression, S/RI 3.75	100	57632	Sub-Tec ball attachment, GH 0, S/RI 4.1–4.5	112
55617	Sub-Dent closed-tray impression, S/RI 4.1	100	57633	Sub-Tec ball attachment, GH 3, S/RI 3.25–3.75	112
55618	Sub-Dent closed-tray impression, S/RI 4.5	100	57634	Sub-Tec ball attachment, GH 3, S/RI 4.1–4.5	112
55551	Sub-Dent closed-tray impression, S/RI 5.5	100	57635	Sub-Tec ball attachment, GH 5, S/RI 3.25–3.75	112
55861	Sub-Dent open-tray impression, S 3.25	100	57636	Sub-Tec ball attachment, GH 5, S/RI 4.1–4.5	112
55540	Sub-Dent open-tray impression, S/RI 3.75	100	57505	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 3.25–3.75	106
55619	Sub-Dent open-tray impression, S/RI 4.1	100	57506	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.1	106
55620	Sub-Dent open-tray impression, S/RI 4.5	100	57507	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.5	106
56500	Sub-Dent open-tray impression, S/RI 5.5	100	57508	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 3.25–3.75	106
57060	Sub-Tec CAD positioner, S/RI 3.25–5.5	98			

INDEX · PRODUCTS LISTED ALPHABETICALLY

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57509	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.1	106	57134	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 3.25–3.75	103
57510	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.5	106	57138	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.1	103
57511	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 3.25–3.75	107	57142	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.5	103
57512	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.1	107	57146	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 5.5	103
57513	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.5	107	57135	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 3.25–3.75	103
57514	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 3.25–3.75	107	57139	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.1	103
57515	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.1	107	57143	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.5	103
57516	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.5	107	57147	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 5.5	103
57517	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 3.25–3.75	107	57132	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 1–2, S/RI 3.25–3.75	103
57518	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.1	107	57136	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.1	103
57519	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.5	107	57140	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.5	103
55526	Sub-Tec Universal no Hex, S/RI 3.25–3.75	104	57144	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 5.5	103
55623	Sub-Tec Universal no Hex, S/RI 4.1	104	57133	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 2.5–4, S/RI 3.25–3.75	103
55528	Sub-Tec Universal no Hex, S/RI 4.5	104	57137	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.1	103
55530	Sub-Tec Universal no Hex, S/RI 5.5	104	57141	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.5	103
55525	Sub-Tec Universal, S/RI 3.25–3.75	104	57145	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 5.5	103
55622	Sub-Tec Universal, S/RI 4.1	104	57116	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 3.25–3.75	102
55527	Sub-Tec Universal, S/RI 4.5	104	57120	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.1	102
55529	Sub-Tec Universal, S/RI 5.5	104	57124	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.5	102
55951	Sub-Tec temporary abutment Ø 7, S/RI 3.25–5.5	101	57128	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 5.5	102
57494	Sub-Tec provisional PEEK abutment, S/RI 3.25–3.75	101	57117	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 3.25–3.75	102
57495	Sub-Tec provisional PEEK abutment, S/RI 4.1–4.5	101	57121	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.1	102
57300	Sub-Tec provisional titanium abutment no Hex, S/RI 3.25–3.75	101	57125	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.5	102
57301	Sub-Tec provisional titanium abutment no Hex, S/RI 4.1	101			
57302	Sub-Tec provisional titanium abutment no Hex, S/RI 4.5	101			
57303	Sub-Tec provisional titanium abutment no Hex, S/RI 5.5	101			
57304	Sub-Tec provisional titanium abutment, S/RI 3.25–3.75	101			
57305	Sub-Tec provisional titanium abutment, S/RI 4.1	101			
57306	Sub-Tec provisional titanium abutment, S/RI 4.5	101			
57307	Sub-Tec provisional titanium abutment, S/RI 5.5	101			

**Note:** Manufacturer notes about trade names, see page 125.

\*<sup>1</sup> New version of the BEGO Semados® RI implants, with Platform Switch design

REF	Article	Page
57129	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5-4,S/RI 5.5	102
	T	
56979	Threadformer, Mini 2.7	62
56980	Threadformer, Mini 2.9	62
56981	Threadformer, Mini 3.1	62
55766	Threadformer, RI 3.25	61
57615	Threadformer, RI 3.75	61
57616	Threadformer, RI 4.1	61
57617	Threadformer, RI 4.5	61
57618	Threadformer, RI 5.5	61
57619	Thread tap, RI 3.75	61
57620	Thread tap, RI 4.1	61
57621	Thread tap, RI 4.5	61
57622	Thread tap, RI 5.5	61
57943	Thread tap, RS/RSX 3.0	58
57944	Thread tap, RS/RSX 3.75	58
57945	Thread tap, RS/RSX 4.1	58
57946	Thread tap, RS/RSX 4.5	58
57947	Thread tap, RS/RSX 5.5	58
57332	Thread tap, S/SC/SCX 3.25	55
57333	Thread tap, S/SC/SCX 3.75	55
57334	Thread tap, S/SC/SCX 4.1	55
57335	Thread tap, S/SC/SCX 4.5	55
57336	Thread tap, S/SC/SCX 5.5	55
57989	TiA, Mini 2.9–3.1 (solid abutment)	117
57988	TiBA, Mini 2.7–3.1 (bar abutment)	118
57464	TJL (training jaw) for mandible	125
57465	TJU (training jaw) for maxilla	125
55817	Trepan drill, Ø4.2 external/Ø3.7 internal	64
55815	Trepan drill, Ø5.0 external/Ø4.1 internal	64
56991	Trepan drill, Ø5.0 external/Ø4.3 internal	64
55816	Trepan drill, Ø6.0 external/Ø5.1 internal	64



# HAPPINESS



A wide range of implants  
for a variety of indications

## SEMADOS® IMPLANTS

A bright smile MADE IN GERMANY

More quality of life for patients  
with a demand-driven system

[www.bego.com](http://www.bego.com)

Partners in Progress

 BEGO



[www.bego.com](http://www.bego.com)



**BEGO Implant Systems GmbH & Co. KG**  
Wilhelm-Herbst-Str. 1 · 28359 Bremen, Germany  
Tel. +49 421 2028-246 · Fax +49 421 2028-265  
E-mail [info@bego-implantology.com](mailto:info@bego-implantology.com) · [www.bego.com](http://www.bego.com)

Want to always be up to date with all BEGO News?  
Register here for the BEGO newsletter: [www.bego.com/newsletter](http://www.bego.com/newsletter)



Products and services shown may not be available in all countries.